

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039642.D
 Acq On : 25 Apr 2023 16:05
 Operator : CG/JU
 Sample : 02433-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE54

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.202	25	28	37	rVB	44850	60893	0.93%	0.107%
2	3.637	99	102	121	rBV	173254	344652	5.27%	0.604%
3	3.854	135	139	146	rVB	23977	41338	0.63%	0.072%
4	4.484	241	246	257	rBV	239579	385121	5.89%	0.675%
5	5.366	394	396	401	rVB2	8906	12206	0.19%	0.021%
6	5.496	415	418	422	rVB	11750	15282	0.23%	0.027%
7	7.001	668	674	692	rBV	102928	292000	4.46%	0.512%
8	7.142	692	698	718	rVV	675079	1202942	18.39%	2.108%
9	7.342	726	732	754	rBV	622277	1167667	17.85%	2.046%
10	7.807	804	811	832	rBV	746170	1333818	20.39%	2.338%
11	8.542	930	936	955	rBV	392950	887144	13.56%	1.555%
12	8.984	1004	1011	1026	rBV	778134	1474843	22.54%	2.585%
13	9.366	1071	1076	1082	rBV6	5985	10120	0.15%	0.018%
14	9.707	1126	1134	1153	rBV	625848	1253216	19.15%	2.196%
15	10.254	1220	1227	1252	rBV	661639	1582124	24.18%	2.773%
16	10.613	1281	1288	1306	rBV	1172919	2004650	30.64%	3.513%
17	10.772	1308	1315	1350	rVV	528479	1348418	20.61%	2.363%
18	11.525	1436	1443	1444	rBV7	4398	6779	0.10%	0.012%
19	12.236	1557	1564	1568	rBV6	9303	19218	0.29%	0.034%
20	13.072	1700	1706	1709	rBV6	4996	8067	0.12%	0.014%
21	13.360	1748	1755	1761	rBV7	8192	13634	0.21%	0.024%
22	13.883	1837	1844	1861	rBV	2209223	3260584	49.84%	5.714%
23	14.160	1884	1891	1910	rBV	2427122	3682177	56.28%	6.453%
24	14.466	1934	1943	1957	rBV	1826968	2723830	41.63%	4.774%
25	14.771	1991	1995	2006	rBV7	21155	85398	1.31%	0.150%
26	14.936	2021	2023	2028	rVB6	5008	7455	0.11%	0.013%
27	15.260	2072	2078	2082	rBV4	7206	12417	0.19%	0.022%
28	15.460	2106	2112	2130	rBV	2990816	4659738	71.22%	8.166%
29	15.601	2130	2136	2150	rBV	864759	1507138	23.04%	2.641%
30	15.836	2171	2176	2190	rVB	38108	74157	1.13%	0.130%
31	16.171	2230	2233	2241	rVV8	3420	6796	0.10%	0.012%
32	16.977	2365	2370	2372	rBV6	4187	6569	0.10%	0.012%
33	17.218	2405	2411	2422	rBV	2253239	3149937	48.14%	5.520%
34	17.318	2422	2428	2445	rVB	3643543	5313026	81.21%	9.311%
35	17.889	2522	2525	2533	rVB9	7633	10197	0.16%	0.018%
36	18.118	2560	2564	2573	rBV2	79340	163965	2.51%	0.287%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039642.D
Acq On : 25 Apr 2023 16:05
Operator : CG/JU
Sample : 02433-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE54

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	18.983	2707	2711	2714	rVB5	8715	11724	0.18%	0.021%
38	19.183	2741	2745	2752	rBV	41887	59137	0.90%	0.104%
39	19.259	2754	2758	2764	rBV	36959	57805	0.88%	0.101%
40	19.401	2778	2782	2792	rBV2	70610	140235	2.14%	0.246%
41	19.542	2803	2806	2810	rBV	22873	29073	0.44%	0.051%
42	19.618	2813	2819	2836	rBV	4773846	6542634	100.00%	11.466%
43	21.418	3120	3125	3139	rBV	2302306	3240003	49.52%	5.678%
44	23.624	3493	3500	3518	rBV2	2862831	5828107	89.08%	10.214%
45	23.777	3519	3526	3540	rVB2	1433989	3024086	46.22%	5.300%




Sum of corrected areas: 57060320

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039642.D
Acq On : 25 Apr 2023 16:05
Operator : CG/JU
Sample : 02433-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

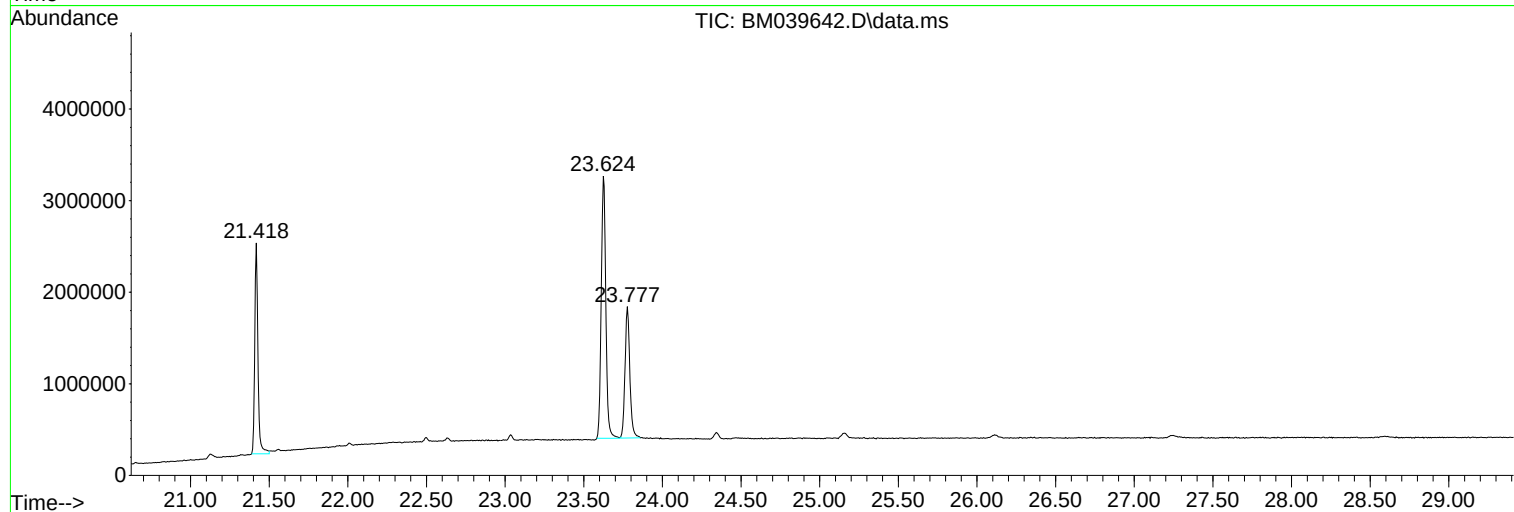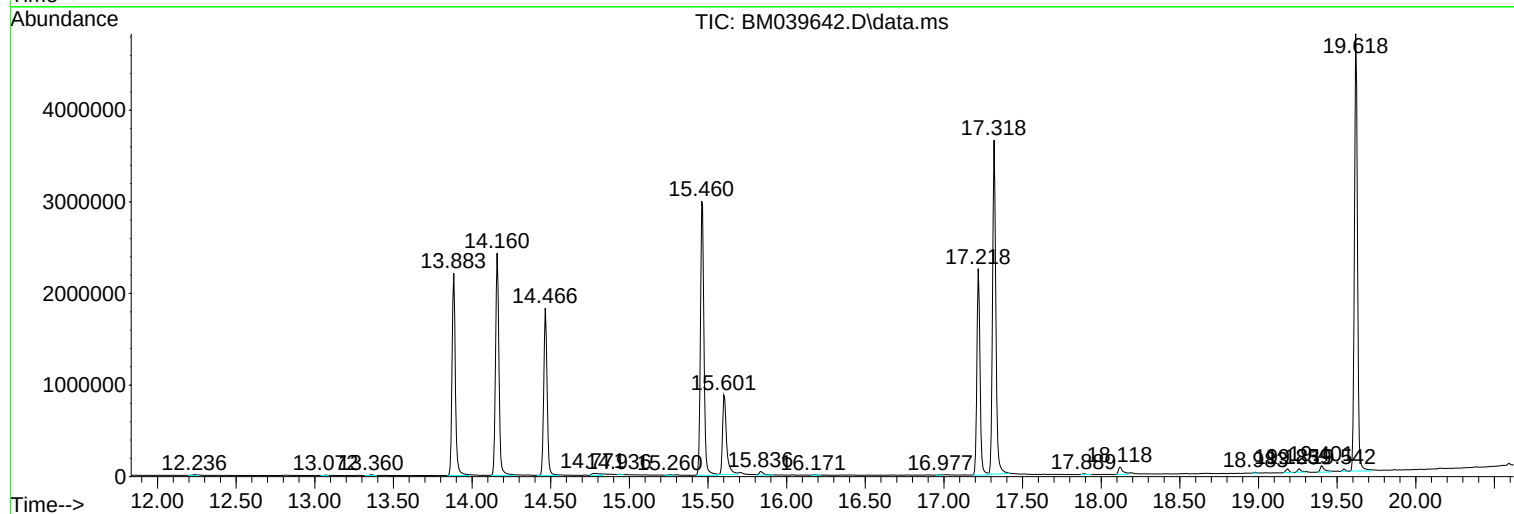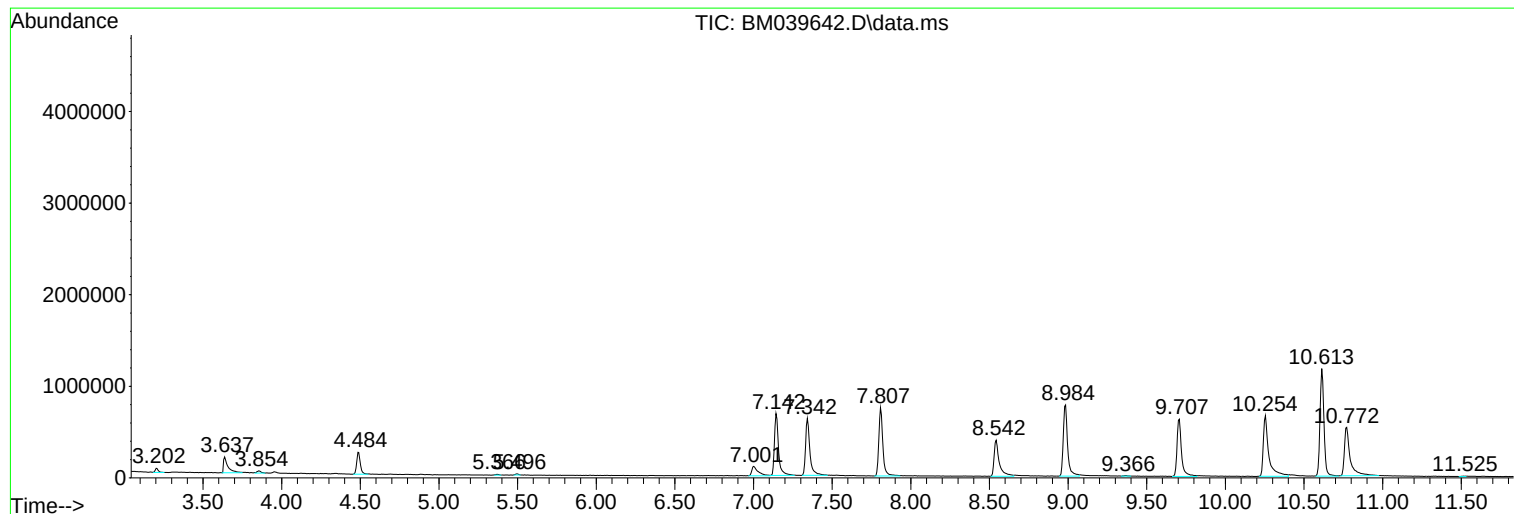

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039642.D
Acq On : 25 Apr 2023 16:05
Operator : CG/JU
Sample : 02433-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039642.D
Acq On : 25 Apr 2023 16:05
Operator : CG/JU
Sample : 02433-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE54

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------