

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039643.D
 Acq On : 25 Apr 2023 16:41
 Operator : CG/JU
 Sample : 02433-20
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039643.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.202	25	28	41	rVB	57992	83788	1.61%	0.161%
2	3.637	99	102	120	rBV	163793	338028	6.50%	0.650%
3	3.854	136	139	147	rVB2	22343	36291	0.70%	0.070%
4	3.954	153	156	162	rVB	15316	23489	0.45%	0.045%
5	4.484	240	246	263	rBV	1668233	2604558	50.10%	5.007%
6	4.878	311	313	318	rBV5	5232	7946	0.15%	0.015%
7	5.366	394	396	402	rVB2	8108	8039	0.15%	0.015%
8	5.495	414	418	427	rVB	13402	24986	0.48%	0.048%
9	7.001	668	674	688	rBV	80291	234675	4.51%	0.451%
10	7.142	692	698	718	rVV	605102	1067393	20.53%	2.052%
11	7.342	726	732	748	rBV	510920	977924	18.81%	1.880%
12	7.807	804	811	824	rBV	686276	1212123	23.32%	2.330%
13	8.542	930	936	959	rBV2	316372	749864	14.42%	1.441%
14	8.984	1004	1011	1033	rBV	663948	1323632	25.46%	2.544%
15	9.707	1126	1134	1152	rBV	499106	1032994	19.87%	1.986%
16	10.254	1220	1227	1254	rBV	511453	1314282	25.28%	2.526%
17	10.613	1281	1288	1305	rVB	1051230	1834290	35.28%	3.526%
18	10.772	1308	1315	1335	rBV	496685	1208507	23.25%	2.323%
19	12.230	1558	1563	1565	rBV5	7932	11149	0.21%	0.021%
20	12.813	1658	1662	1666	rBV7	4207	5816	0.11%	0.011%
21	13.071	1700	1706	1709	rBV6	4535	7791	0.15%	0.015%
22	13.277	1737	1741	1748	rVB9	4567	8761	0.17%	0.017%
23	13.360	1748	1755	1760	rBV	15086	25604	0.49%	0.049%
24	13.883	1837	1844	1860	rBV	1768115	2700424	51.95%	5.191%
25	14.160	1884	1891	1909	rBV	2127384	3196154	61.48%	6.144%
26	14.466	1936	1943	1956	rBV	1689013	2497731	48.05%	4.801%
27	14.713	1979	1985	1987	rBV7	4143	6298	0.12%	0.012%
28	14.795	1992	1999	2002	rBV7	13478	34947	0.67%	0.067%
29	15.260	2075	2078	2081	rBV	4545	5776	0.11%	0.011%
30	15.460	2106	2112	2131	rBV	2579139	4037221	77.66%	7.761%
31	15.601	2131	2136	2151	rVV	579367	1102169	21.20%	2.119%
32	15.701	2151	2153	2159	rVB4	16259	27758	0.53%	0.053%
33	15.836	2171	2176	2188	rVB2	51395	94570	1.82%	0.182%
34	16.042	2207	2211	2216	rVB8	4190	6889	0.13%	0.013%
35	16.171	2230	2233	2240	rVB8	5351	8323	0.16%	0.016%
36	16.883	2348	2354	2355	rBV6	3783	5211	0.10%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039643.D
 Acq On : 25 Apr 2023 16:41
 Operator : CG/JU
 Sample : 02433-20
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE55

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	17.007	2373	2375	2381	rVB6	6240	9919	0.19%	0.019%
38	17.218	2404	2411	2422	rBV	1963873	2843440	54.70%	5.466%
39	17.318	2422	2428	2446	rVV	3218434	4719898	90.79%	9.073%
40	17.706	2491	2494	2497	rBV5	7377	8566	0.16%	0.016%
41	17.889	2521	2525	2529	rBV7	8357	13102	0.25%	0.025%
42	18.118	2559	2564	2573	rBV	114672	218691	4.21%	0.420%
43	18.189	2574	2576	2582	rVB	24461	32912	0.63%	0.063%
44	18.401	2610	2612	2619	rVB7	10295	14280	0.27%	0.027%
45	19.042	2719	2721	2725	rVB4	8548	8412	0.16%	0.016%
46	19.183	2741	2745	2752	rBV2	36649	57783	1.11%	0.111%
47	19.259	2754	2758	2764	rBV	32803	59118	1.14%	0.114%
48	19.400	2778	2782	2793	rBV2	97134	192469	3.70%	0.370%
49	19.542	2804	2806	2810	rVB3	22626	23493	0.45%	0.045%
50	19.618	2813	2819	2833	rBV	3725378	5198567	100.00%	9.993%
51	19.859	2857	2860	2869	rBV4	20610	33962	0.65%	0.065%
52	21.130	3071	3076	3085	rBV5	85069	219745	4.23%	0.422%
53	21.418	3120	3125	3143	rBV	2007267	2941074	56.57%	5.654%
54	23.624	3493	3500	3514	rBV2	2368905	4908545	94.42%	9.436%
55	23.777	3520	3526	3540	rVB2	1259980	2651404	51.00%	5.097%




Sum of corrected areas: 52020781

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039643.D
Acq On : 25 Apr 2023 16:41
Operator : CG/JU
Sample : 02433-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

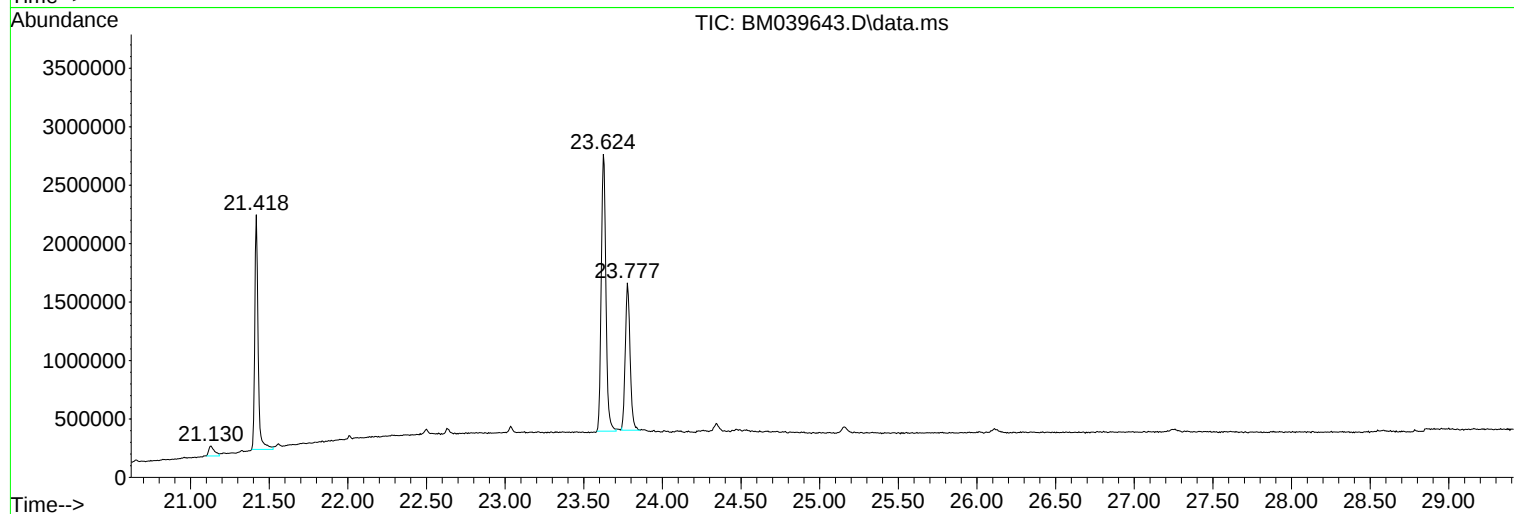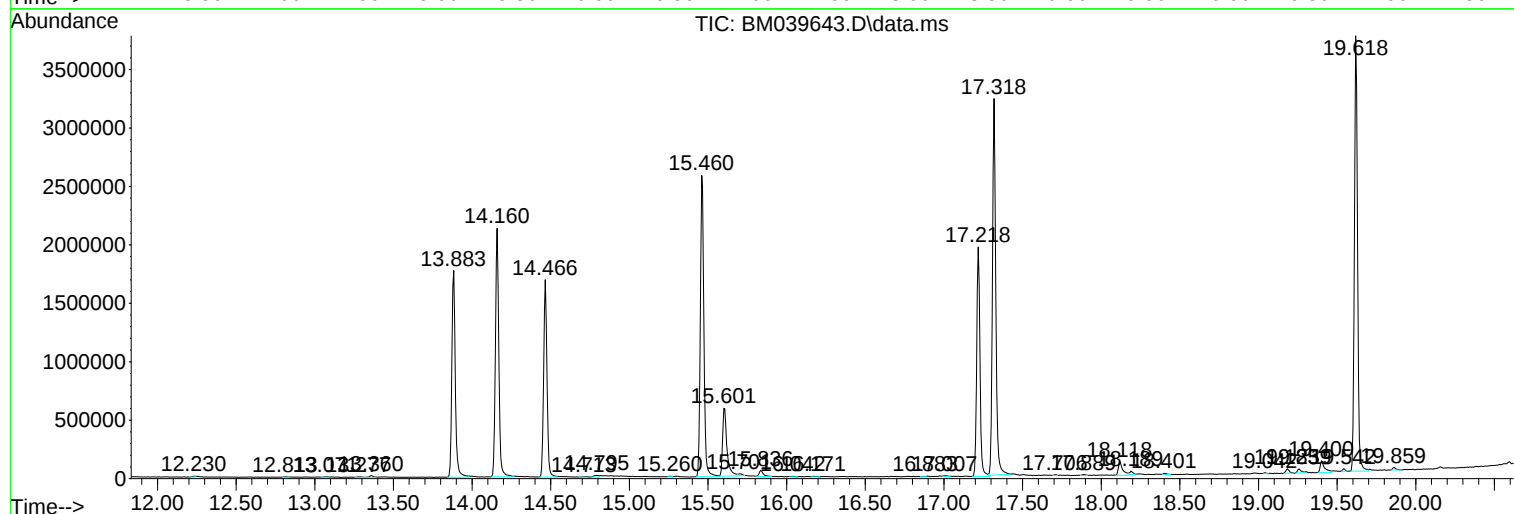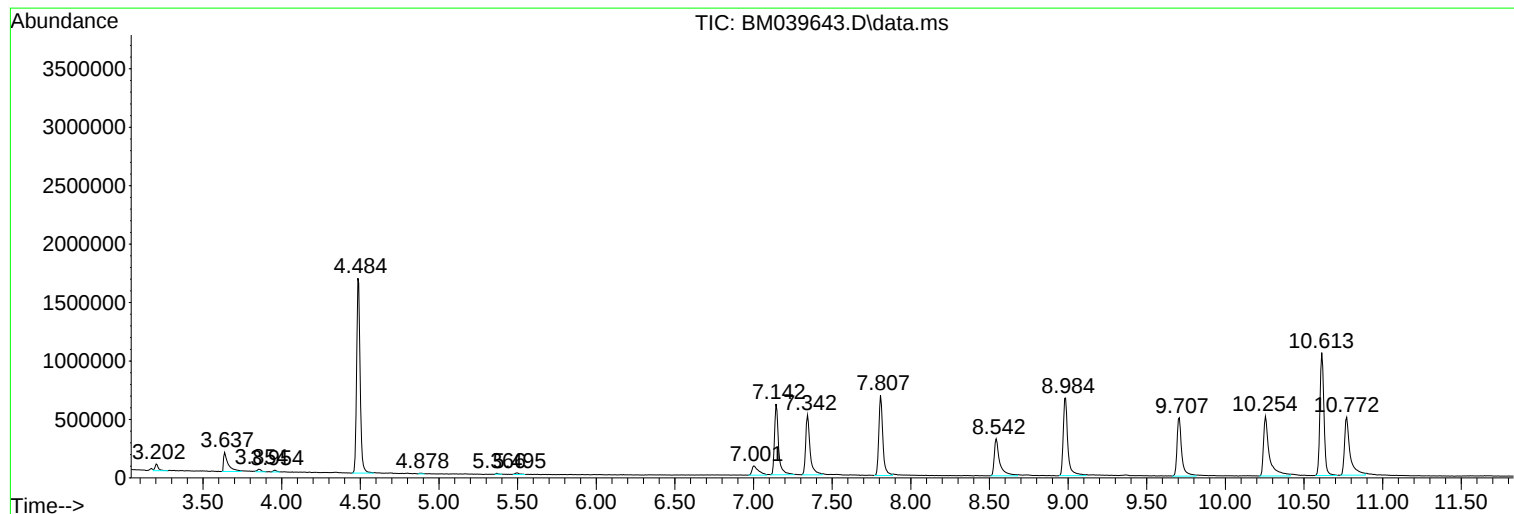

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039643.D
Acq On : 25 Apr 2023 16:41
Operator : CG/JU
Sample : 02433-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039643.D
Acq On : 25 Apr 2023 16:41
Operator : CG/JU
Sample : 02433-20
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE55

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------