

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039644.D
 Acq On : 25 Apr 2023 17:17
 Operator : CG/JU
 Sample : 02433-21
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.202	25	28	38	rVB	44995	66653	1.14%	0.124%
2	3.637	100	102	118	rBV	203736	389485	6.67%	0.726%
3	3.855	136	139	149	rVB	26456	40954	0.70%	0.076%
4	3.955	154	156	166	rVB3	14614	23986	0.41%	0.045%
5	4.490	241	247	255	rBV	185808	296485	5.08%	0.552%
6	5.372	394	397	403	rVB	9886	14571	0.25%	0.027%
7	5.490	415	417	421	rBV	12579	16185	0.28%	0.030%
8	7.001	668	674	688	rBV	105584	295162	5.06%	0.550%
9	7.143	692	698	721	rVB	682760	1208203	20.70%	2.251%
10	7.343	726	732	755	rVB	608041	1142709	19.57%	2.129%
11	7.807	804	811	824	rBV	704180	1243142	21.29%	2.316%
12	8.542	929	936	961	rBV	397207	914563	15.67%	1.704%
13	8.984	1003	1011	1030	rBV	770129	1507819	25.83%	2.809%
14	9.366	1072	1076	1081	rVB3	8277	12733	0.22%	0.024%
15	9.701	1126	1133	1160	rBV	590796	1199384	20.55%	2.234%
16	10.254	1220	1227	1246	rBV	622660	1474455	25.26%	2.747%
17	10.613	1281	1288	1305	rBV	1103552	1886903	32.32%	3.515%
18	10.766	1308	1314	1340	rBV	558717	1393524	23.87%	2.596%
19	12.236	1557	1564	1573	rBV4	10802	30425	0.52%	0.057%
20	12.819	1658	1663	1670	rBV7	4403	8367	0.14%	0.016%
21	13.077	1701	1707	1710	rBV5	7832	12759	0.22%	0.024%
22	13.360	1749	1755	1761	rVB7	7059	14160	0.24%	0.026%
23	13.883	1837	1844	1862	rBV	2075614	3068506	52.56%	5.716%
24	14.160	1882	1891	1909	rBV2	2384565	3636882	62.30%	6.775%
25	14.466	1936	1943	1960	rBV	1715801	2532170	43.38%	4.717%
26	14.783	1991	1997	2001	rBV6	17473	42666	0.73%	0.079%
27	15.260	2072	2078	2082	rBV2	9995	15151	0.26%	0.028%
28	15.295	2082	2084	2090	rVB3	9325	13651	0.23%	0.025%
29	15.460	2106	2112	2131	rBV	2837208	4406763	75.49%	8.210%
30	15.601	2131	2136	2151	rBV	666156	1216399	20.84%	2.266%
31	15.836	2171	2176	2190	rVB	37430	69802	1.20%	0.130%
32	16.171	2229	2233	2240	rBV3	18548	36905	0.63%	0.069%
33	16.895	2353	2356	2360	rBV6	4144	7029	0.12%	0.013%
34	16.971	2364	2369	2372	rBV2	17044	26225	0.45%	0.049%
35	17.012	2373	2376	2381	rVB5	9158	14930	0.26%	0.028%
36	17.218	2405	2411	2422	rBV	2031042	2940626	50.37%	5.478%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039644.D
 Acq On : 25 Apr 2023 17:17
 Operator : CG/JU
 Sample : 02433-21
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE56

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	17.318	2422	2428	2445	rVB	3344528	4965641	85.06%	9.251%
38	17.507	2458	2460	2465	rVB4	7024	10866	0.19%	0.020%
39	17.712	2491	2495	2501	rBV5	9182	11893	0.20%	0.022%
40	17.889	2521	2525	2532	rBV6	13162	23674	0.41%	0.044%
41	18.124	2561	2565	2573	rBV4	27942	62367	1.07%	0.116%
42	18.195	2573	2577	2582	rVB	18572	30279	0.52%	0.056%
43	18.407	2610	2613	2618	rVB5	5916	7485	0.13%	0.014%
44	19.183	2741	2745	2753	rBV2	38120	54948	0.94%	0.102%
45	19.259	2754	2758	2763	rBV	36096	54825	0.94%	0.102%
46	19.406	2780	2783	2788	rBV6	16497	29525	0.51%	0.055%
47	19.542	2803	2806	2810	rBV2	20389	25787	0.44%	0.048%
48	19.618	2813	2819	2837	rBV	4244085	5837757	100.00%	10.875%
49	21.418	3120	3125	3140	rBV	2150648	3076566	52.70%	5.731%
50	23.624	3493	3500	3518	rBV2	2622883	5404214	92.57%	10.068%
51	23.777	3520	3526	3540	rVB2	1301191	2862354	49.03%	5.332%




Sum of corrected areas: 53678513

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039644.D
Acq On : 25 Apr 2023 17:17
Operator : CG/JU
Sample : 02433-21
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

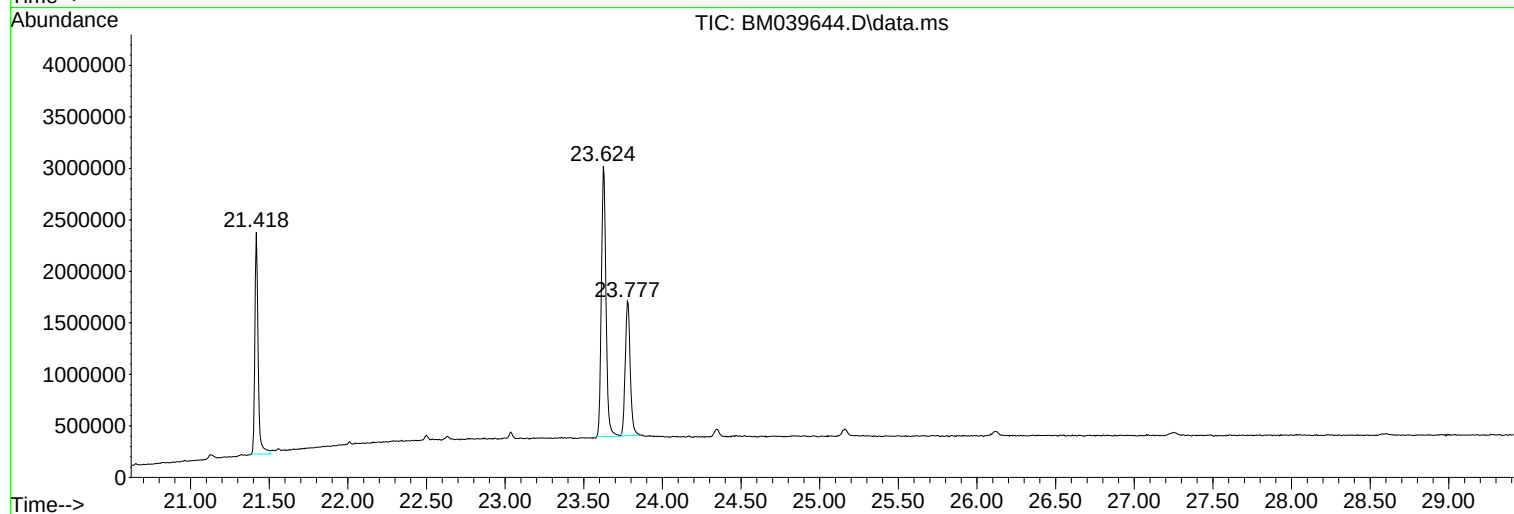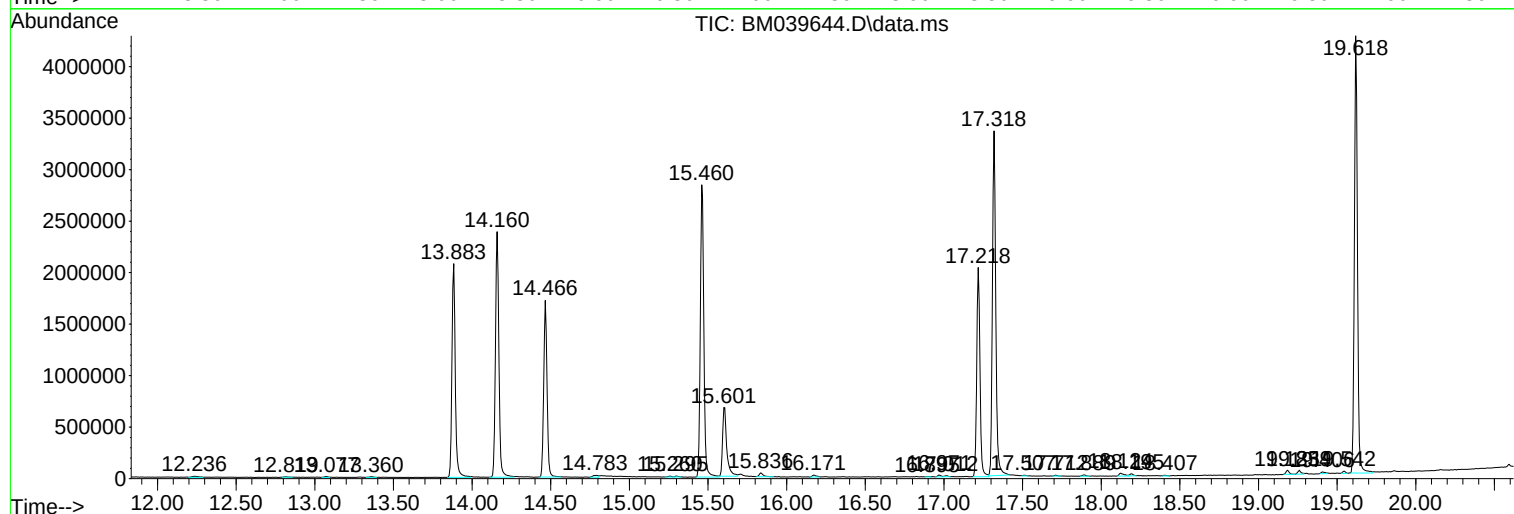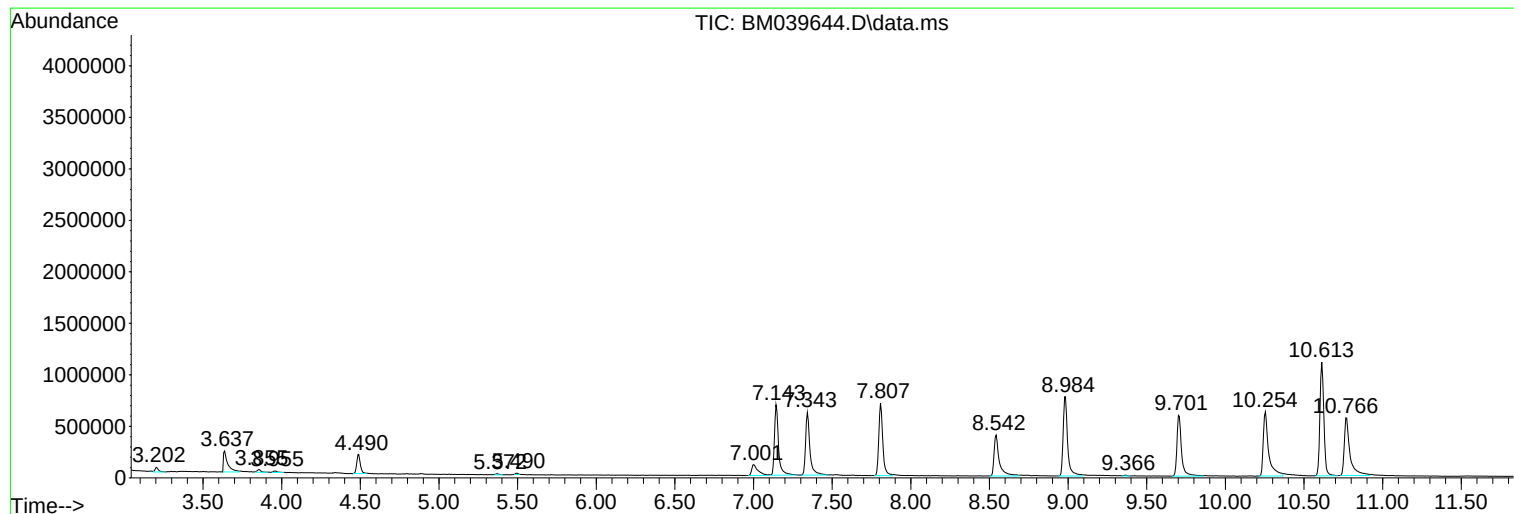

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039644.D
Acq On : 25 Apr 2023 17:17
Operator : CG/JU
Sample : 02433-21
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039644.D
Acq On : 25 Apr 2023 17:17
Operator : CG/JU
Sample : 02433-21
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE56

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc