

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039649.D
 Acq On : 25 Apr 2023 20:17
 Operator : CG/JU
 Sample : 02488-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039649.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.172	19	23	26	rBV	39810	58000	0.87%	0.100%
2	3.201	26	28	32	rVB	38889	42955	0.65%	0.074%
3	3.648	101	104	116	rBV	53219	119453	1.80%	0.205%
4	3.854	135	139	145	rVB2	24733	40461	0.61%	0.070%
5	3.954	153	156	164	rVB2	14373	22172	0.33%	0.038%
6	4.490	243	247	256	rVB2	26526	46181	0.69%	0.079%
7	5.372	393	397	401	rVB	9738	14518	0.22%	0.025%
8	5.495	414	418	424	rBV	14729	23064	0.35%	0.040%
9	7.001	668	674	692	rBV	106308	291058	4.38%	0.500%
10	7.142	692	698	719	rBV	814677	1408795	21.18%	2.421%
11	7.342	725	732	753	rBV	718476	1335253	20.07%	2.294%
12	7.807	804	811	830	rBV	662652	1189423	17.88%	2.044%
13	8.536	929	935	954	rBV	451631	993163	14.93%	1.707%
14	8.978	1004	1010	1030	rBV	967101	1804845	27.13%	3.101%
15	9.366	1071	1076	1080	rVB3	8122	11752	0.18%	0.020%
16	9.701	1126	1133	1149	rBV	764838	1473243	22.15%	2.532%
17	10.254	1220	1227	1255	rBV	741370	1860160	27.96%	3.196%
18	10.613	1280	1288	1302	rBV	1007995	1751071	26.32%	3.009%
19	10.772	1308	1315	1340	rBV	278214	781879	11.75%	1.344%
20	11.866	1493	1501	1505	rVB7	5008	8638	0.13%	0.015%
21	12.042	1525	1531	1536	rVB7	3470	8822	0.13%	0.015%
22	12.236	1557	1564	1573	rBV3	12166	30820	0.46%	0.053%
23	13.883	1837	1844	1858	rBV	2394706	3546739	53.31%	6.094%
24	14.160	1884	1891	1909	rBV	2837694	4238588	63.71%	7.283%
25	14.465	1936	1943	1956	rBV	1575077	2351009	35.34%	4.040%
26	14.783	1991	1997	2003	rBV6	18519	58265	0.88%	0.100%
27	15.459	2106	2112	2131	rBV	3493441	5395091	81.10%	9.271%
28	15.601	2131	2136	2151	rVV	921605	1588475	23.88%	2.730%
29	15.706	2151	2154	2159	rVB4	21508	36472	0.55%	0.063%
30	15.836	2170	2176	2186	rVB	45112	84960	1.28%	0.146%
31	16.254	2243	2247	2253	rBV8	4197	7148	0.11%	0.012%
32	17.218	2404	2411	2422	rBV	1986186	2797485	42.05%	4.807%
33	17.318	2422	2428	2448	rVB	4040341	5803196	87.23%	9.972%
34	17.618	2477	2479	2486	rVB6	6897	7337	0.11%	0.013%
35	17.889	2522	2525	2530	rVB7	7092	10611	0.16%	0.018%
36	18.118	2560	2564	2574	rBV2	52967	111872	1.68%	0.192%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039649.D
 Acq On : 25 Apr 2023 20:17
 Operator : CG/JU
 Sample : 02488-04
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE60

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	18.189	2574	2576	2583	rVB3	7951	11148	0.17%	0.019%
38	18.977	2707	2710	2716	rBV7	10642	17345	0.26%	0.030%
39	19.183	2741	2745	2752	rBV2	47781	72566	1.09%	0.125%
40	19.259	2754	2758	2770	rVV2	36657	72573	1.09%	0.125%
41	19.406	2779	2783	2789	rBV6	23653	48503	0.73%	0.083%
42	19.542	2803	2806	2811	rBV4	17541	22317	0.34%	0.038%
43	19.618	2813	2819	2832	rBV	4788767	6652583	100.00%	11.431%
44	21.124	3071	3075	3086	rBV6	67933	187239	2.81%	0.322%
45	21.418	3120	3125	3136	rBV	2005522	2839217	42.68%	4.879%
46	23.624	3493	3500	3515	rBV2	3025570	6146428	92.39%	10.562%
47	23.777	3520	3526	3544	rVB2	1259440	2773211	41.69%	4.765%




Sum of corrected areas: 58196104

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039649.D
Acq On : 25 Apr 2023 20:17
Operator : CG/JU
Sample : 02488-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

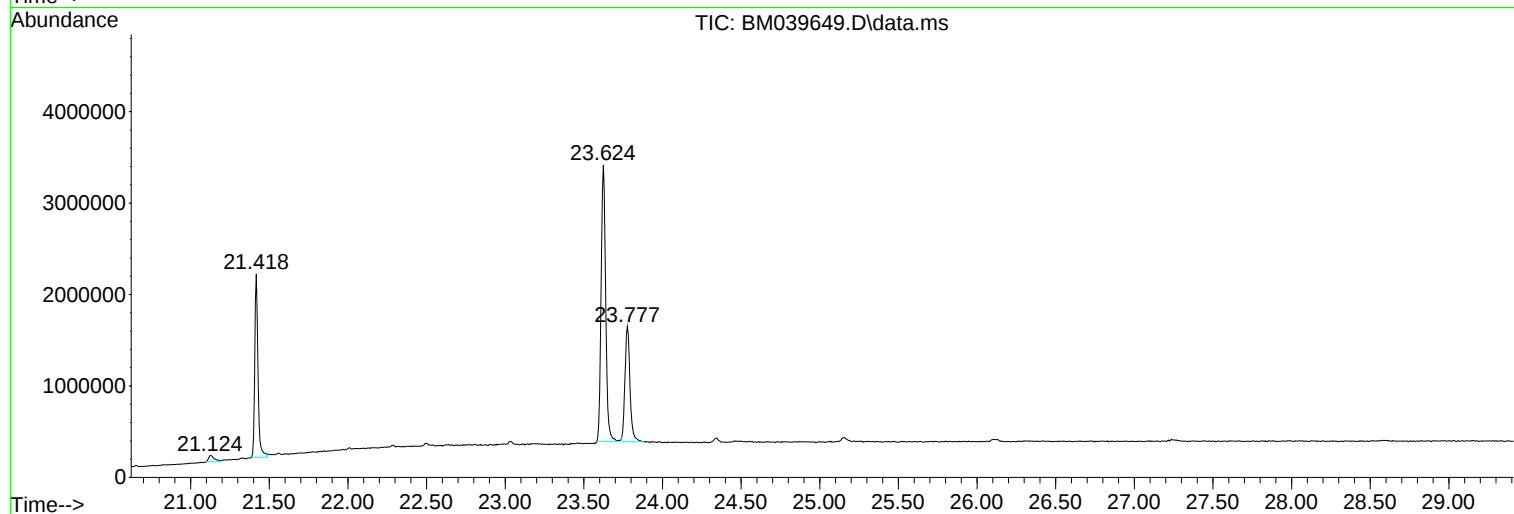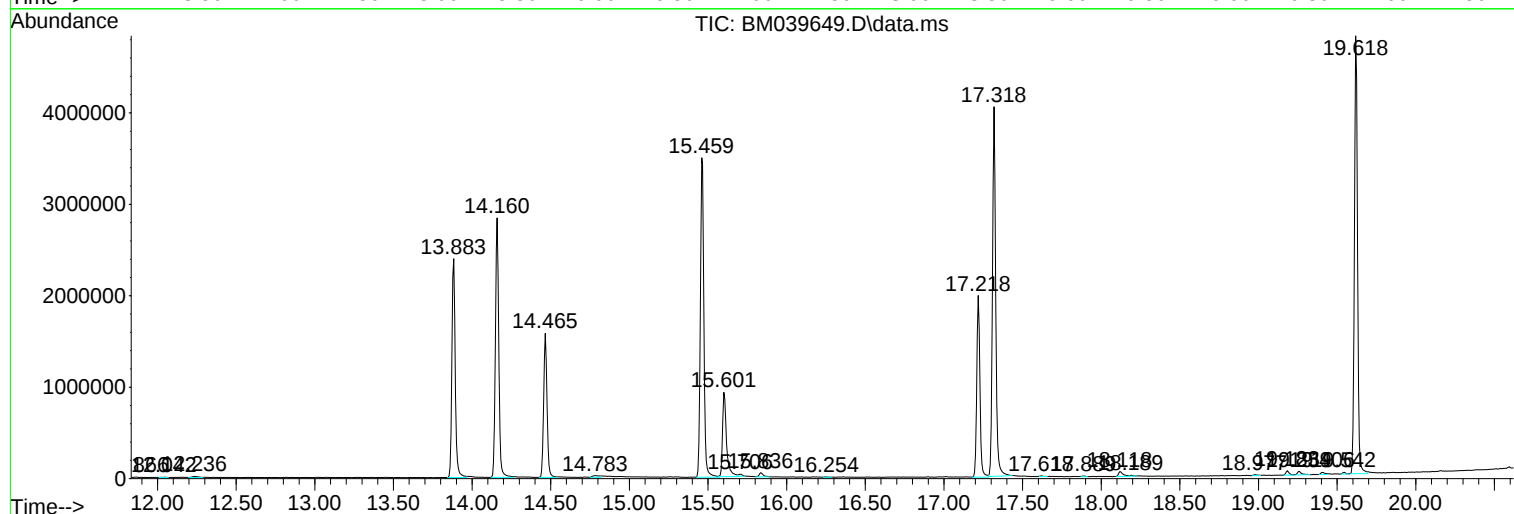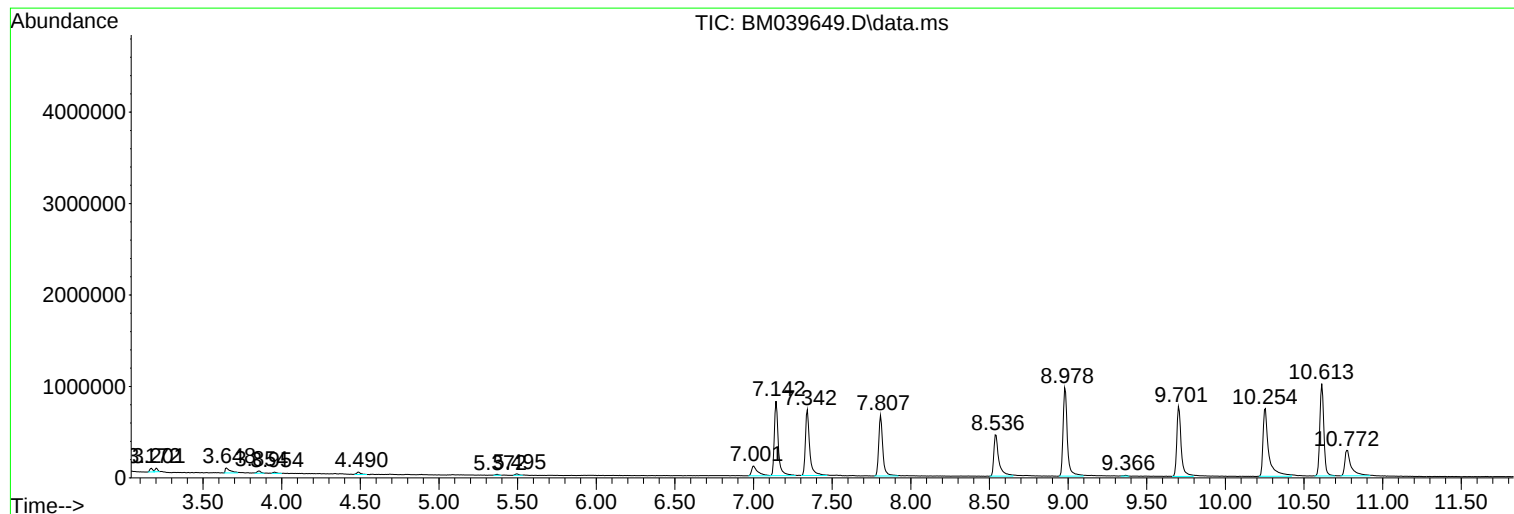

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039649.D
Acq On : 25 Apr 2023 20:17
Operator : CG/JU
Sample : 02488-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039649.D
Acq On : 25 Apr 2023 20:17
Operator : CG/JU
Sample : 02488-04
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE60

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc