

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039651.D
 Acq On : 25 Apr 2023 22:05
 Operator : CG/JU
 Sample : PB152398BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK398

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.201	25	28	37	rVB	58515	84362	1.51%	0.146%
2	3.625	97	100	127	rBV	705369	1281731	22.88%	2.222%
3	6.989	666	672	692	rBV	719894	1450443	25.89%	2.514%
4	7.142	692	698	721	rVB	786636	1362098	24.31%	2.361%
5	7.336	725	731	751	rBV	881063	1607410	28.69%	2.787%
6	7.807	804	811	825	rBV	751811	1316794	23.50%	2.283%
7	8.536	928	935	962	rBV	946285	1881287	33.58%	3.261%
8	8.978	1001	1010	1028	rBV	754538	1426274	25.46%	2.473%
9	9.701	1127	1133	1152	rBV	622068	1220423	21.78%	2.116%
10	9.825	1152	1154	1161	rVB8	6354	10157	0.18%	0.018%
11	10.248	1220	1226	1254	rBV	681217	1633439	29.15%	2.832%
12	10.613	1280	1288	1305	rBV	1026356	1779771	31.77%	3.085%
13	10.766	1307	1314	1334	rBV	724404	1668608	29.78%	2.893%
14	12.242	1561	1565	1567	rBV4	6498	10299	0.18%	0.018%
15	13.360	1751	1755	1762	rBV9	3179	7103	0.13%	0.012%
16	13.883	1837	1844	1860	rBV	2028556	3122753	55.74%	5.414%
17	14.160	1884	1891	1911	rBV	2412359	3740926	66.77%	6.485%
18	14.465	1936	1943	1960	rBV	1817075	2716214	48.48%	4.709%
19	14.730	1982	1988	2011	rBV3	157936	820449	14.64%	1.422%
20	15.459	2106	2112	2131	rBV	2922586	4524153	80.75%	7.843%
21	15.601	2131	2136	2151	rBV	689866	1282330	22.89%	2.223%
22	17.218	2405	2411	2422	rBV	2138602	3114013	55.58%	5.398%
23	17.318	2422	2428	2453	rVB2	3196759	4827669	86.17%	8.369%
24	19.183	2741	2745	2750	rBV3	32230	49647	0.89%	0.086%
25	19.259	2754	2758	2766	rBV	29168	46154	0.82%	0.080%
26	19.618	2813	2819	2843	rBV	3941249	5602616	100.00%	9.713%
27	21.418	3120	3125	3144	rBV	2112750	3191706	56.97%	5.533%
28	23.624	3493	3500	3517	rBV2	2345234	4926635	87.93%	8.541%
29	23.777	3520	3526	3541	rVB2	1332584	2978529	53.16%	5.164%




Sum of corrected areas: 57683993

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039651.D
Acq On : 25 Apr 2023 22:05
Operator : CG/JU
Sample : PB152398BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

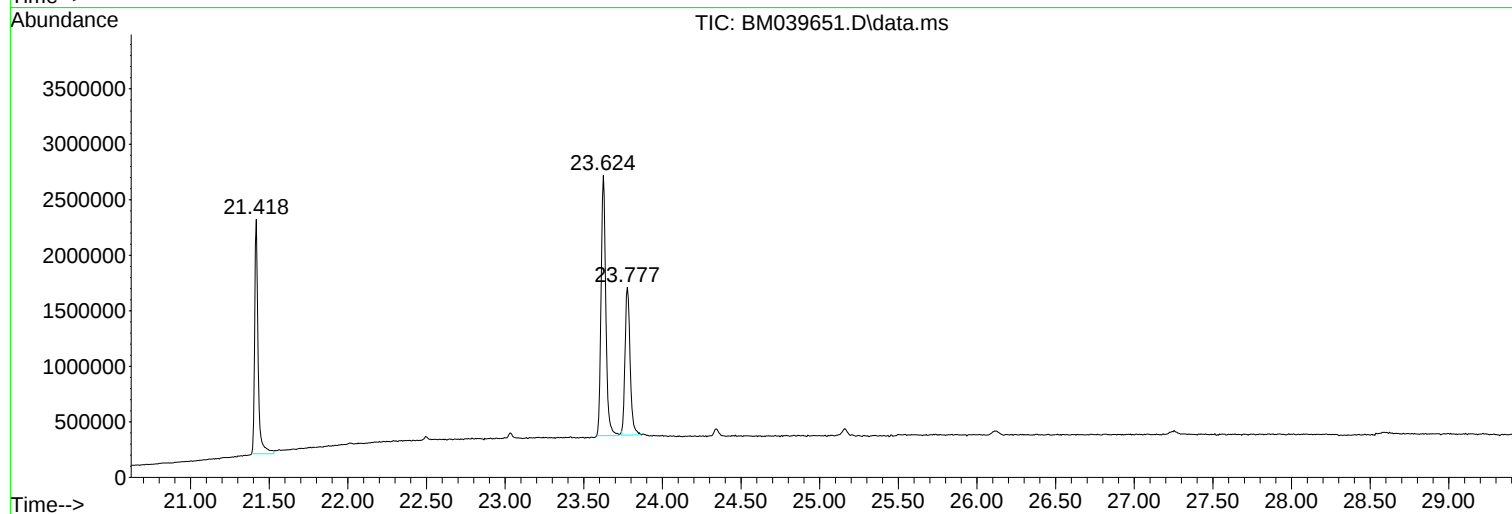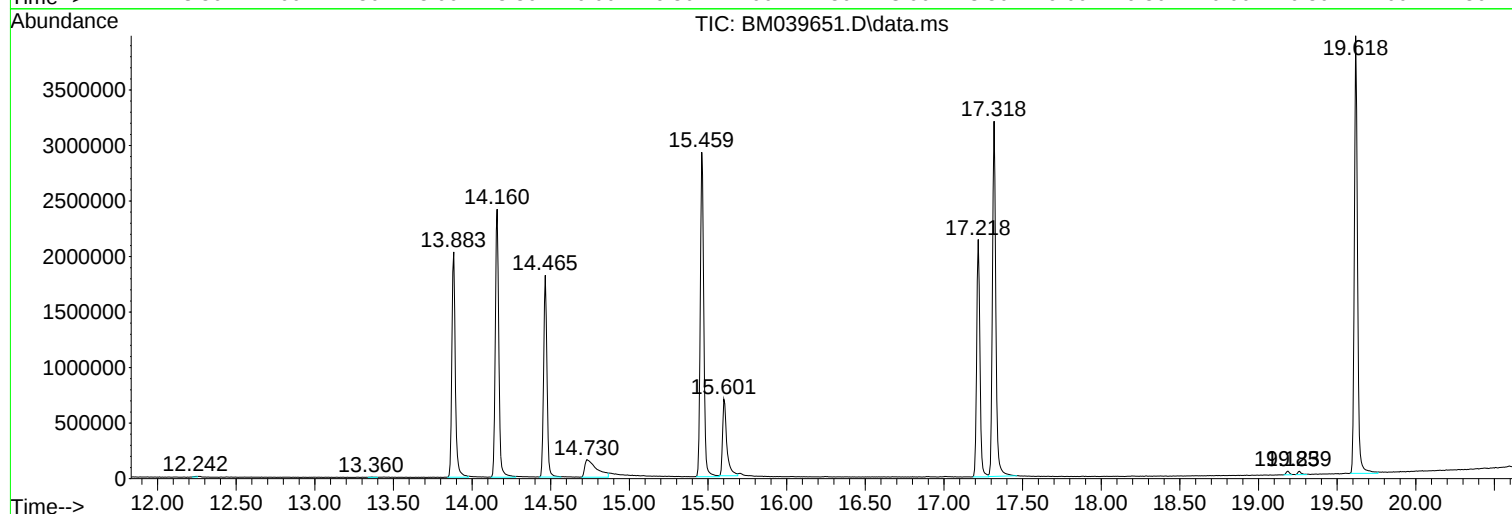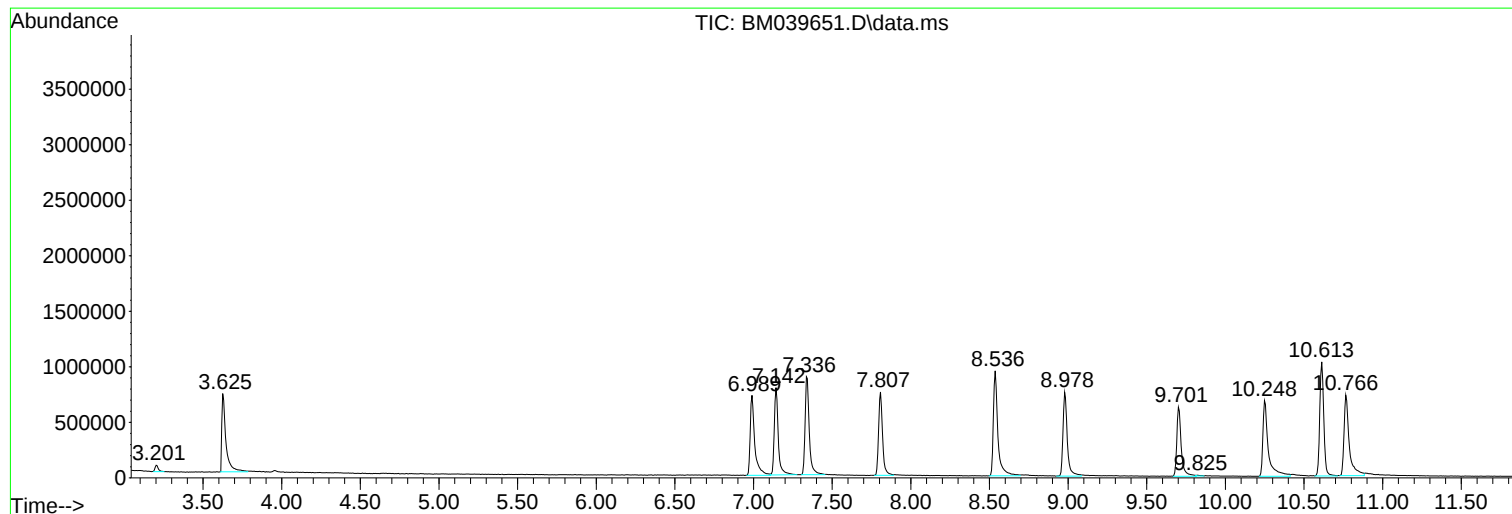

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039651.D
Acq On : 25 Apr 2023 22:05
Operator : CG/JU
Sample : PB152398BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039651.D
Acq On : 25 Apr 2023 22:05
Operator : CG/JU
Sample : PB152398BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK398

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc