

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039653.D
 Acq On : 25 Apr 2023 23:17
 Operator : CG/JU
 Sample : 02488-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.172	19	23	25	rBV3	22763	29998	0.40%	0.045%
2	3.201	25	28	37	rVB	53454	82016	1.10%	0.123%
3	3.648	103	104	112	rBV	41501	78468	1.05%	0.118%
4	3.860	136	140	146	rVB2	26607	44090	0.59%	0.066%
5	3.954	154	156	161	rVB	13241	15365	0.21%	0.023%
6	4.484	240	246	267	rBV	2413711	3672870	49.34%	5.519%
7	5.366	392	396	404	rVB	8051	16158	0.22%	0.024%
8	5.495	414	418	425	rBV	14705	21651	0.29%	0.033%
9	6.995	668	673	690	rBV	143448	359213	4.83%	0.540%
10	7.142	692	698	713	rBV	836171	1388878	18.66%	2.087%
11	7.342	725	732	749	rBV	789722	1476522	19.83%	2.219%
12	7.807	804	811	832	rBV	759750	1354505	18.19%	2.035%
13	8.536	929	935	955	rBV	545746	1169289	15.71%	1.757%
14	8.978	1004	1010	1027	rBV	1008467	1861330	25.00%	2.797%
15	9.366	1071	1076	1081	rVB4	11406	19118	0.26%	0.029%
16	9.701	1126	1133	1151	rBV	819717	1555192	20.89%	2.337%
17	10.248	1219	1226	1250	rBV	833060	2049916	27.54%	3.080%
18	10.613	1280	1288	1304	rBV	1181170	2032600	27.30%	3.054%
19	10.772	1309	1315	1338	rBV	237392	702321	9.43%	1.055%
20	11.001	1349	1354	1363	rVB5	13062	30986	0.42%	0.047%
21	12.236	1559	1564	1573	rVB4	10256	26020	0.35%	0.039%
22	13.360	1750	1755	1760	rBV5	6074	8853	0.12%	0.013%
23	13.883	1834	1844	1858	rBV	2520000	3798547	51.02%	5.708%
24	14.160	1883	1891	1911	rBV	2956696	4466923	60.00%	6.712%
25	14.465	1936	1943	1961	rBV	1834316	2713102	36.44%	4.077%
26	14.771	1989	1995	2004	rBV4	28061	109394	1.47%	0.164%
27	15.459	2105	2112	2130	rBV	3768429	5615029	75.42%	8.437%
28	15.601	2130	2136	2150	rBV	1032937	1686171	22.65%	2.534%
29	15.836	2170	2176	2188	rVB	68303	127425	1.71%	0.191%
30	16.171	2230	2233	2239	rBV8	5009	9898	0.13%	0.015%
31	17.218	2405	2411	2422	rBV	2193113	3119299	41.90%	4.687%
32	17.318	2422	2428	2455	rVV	4151831	6181587	83.03%	9.289%
33	17.506	2458	2460	2468	rVB6	7136	13618	0.18%	0.020%
34	17.883	2522	2524	2528	rVB4	8610	10030	0.13%	0.015%
35	18.118	2559	2564	2574	rBV	110424	211059	2.84%	0.317%
36	18.971	2707	2709	2713	rBV5	8467	11696	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039653.D
Acq On : 25 Apr 2023 23:17
Operator : CG/JU
Sample : 02488-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE61

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	19.183	2741	2745	2750	rBV2	50265	72256	0.97%	0.109%
38	19.259	2754	2758	2762	rBV	43404	68130	0.92%	0.102%
39	19.400	2778	2782	2790	rBV3	43496	82970	1.11%	0.125%
40	19.542	2803	2806	2809	rVB3	25008	25023	0.34%	0.038%
41	19.618	2813	2819	2829	rBV	5683077	7444572	100.00%	11.186%
42	21.130	3071	3076	3085	rBV4	89920	216420	2.91%	0.325%
43	21.412	3119	3124	3140	rBV	2203271	3216876	43.21%	4.834%
44	23.624	3492	3500	3516	rBV2	3094759	6440360	86.51%	9.677%
45	23.771	3519	3525	3540	rVB2	1398480	2915225	39.16%	4.380%




Sum of corrected areas: 66550969

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039653.D
Acq On : 25 Apr 2023 23:17
Operator : CG/JU
Sample : 02488-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

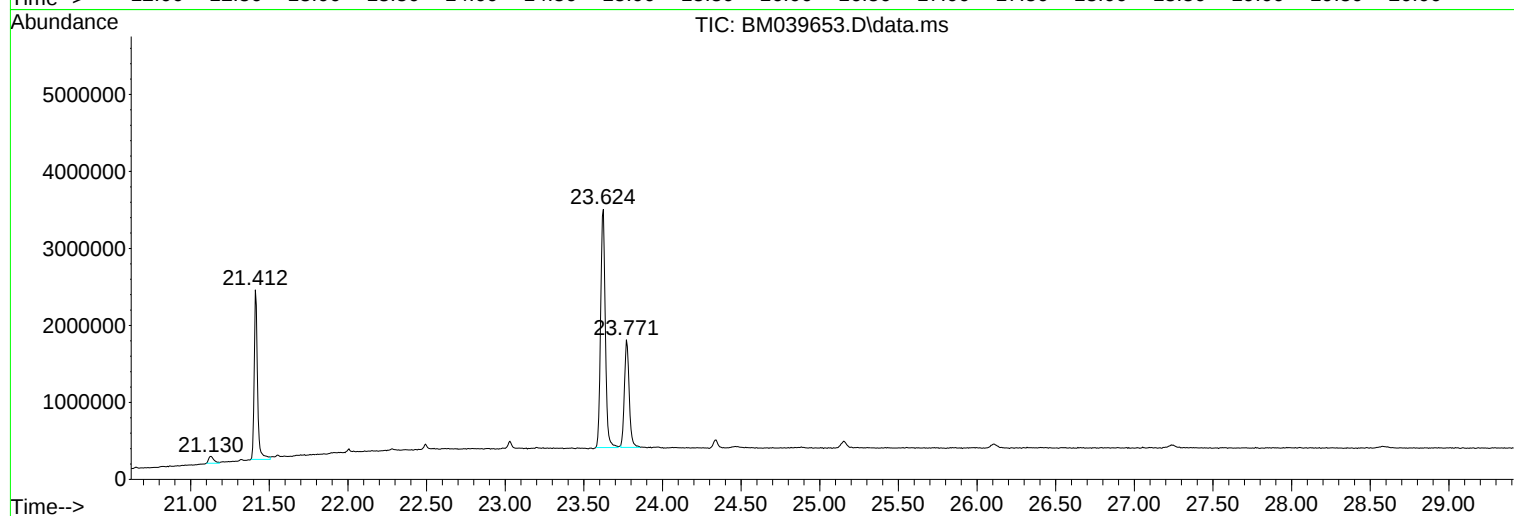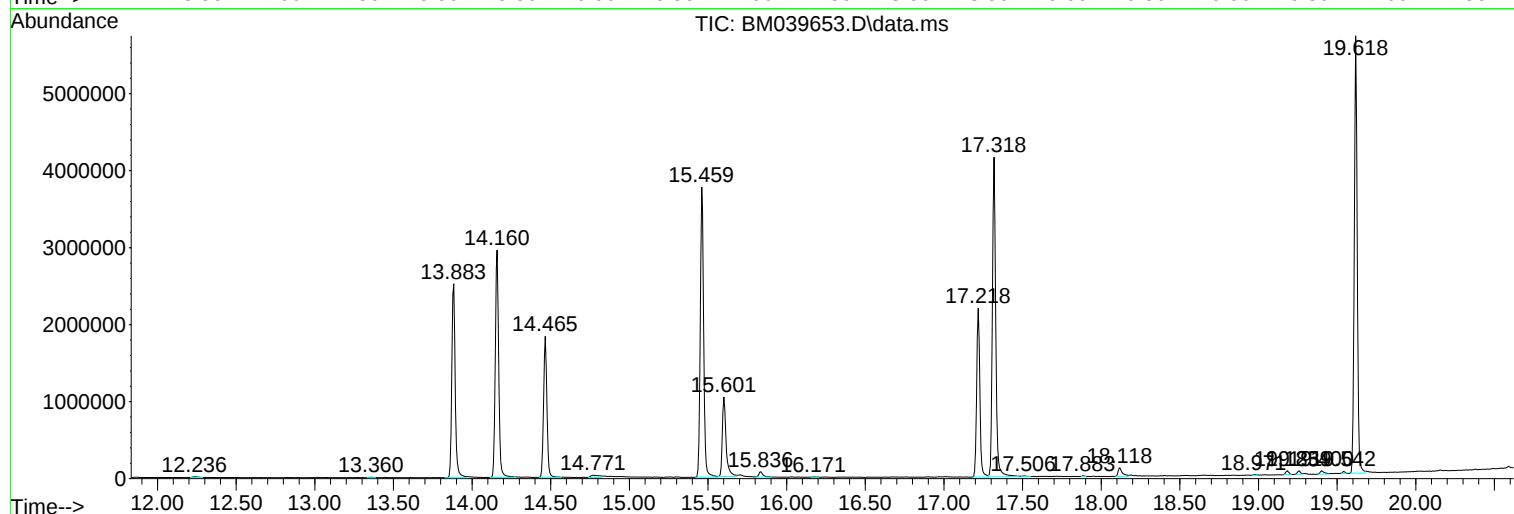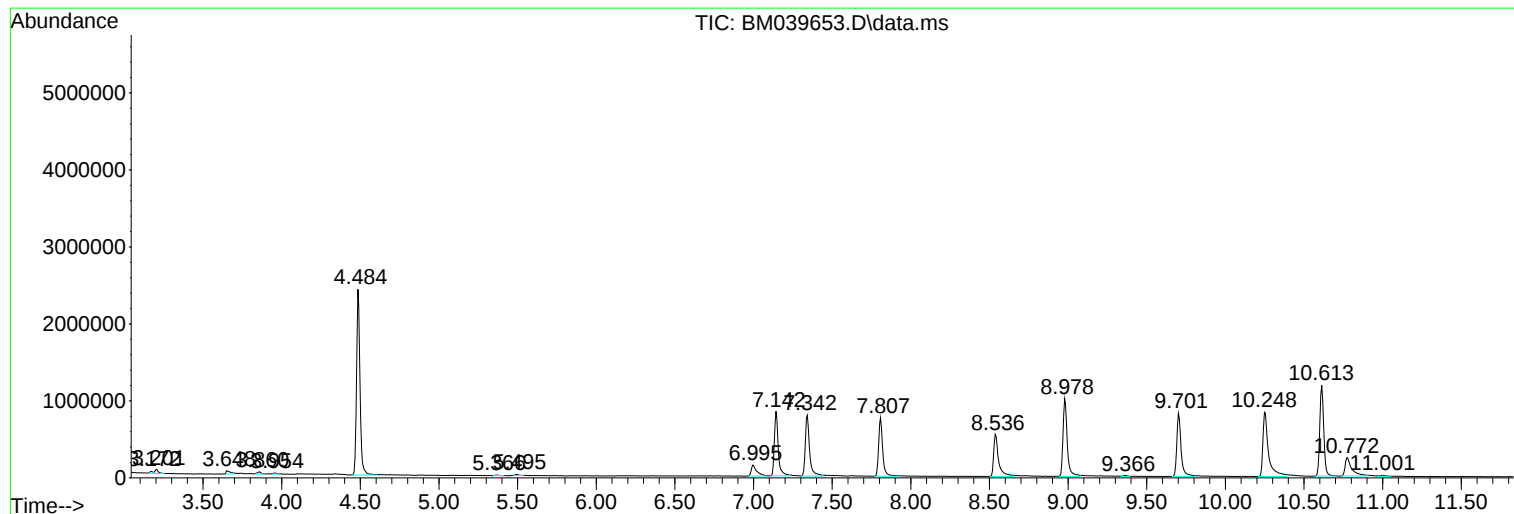

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039653.D
Acq On : 25 Apr 2023 23:17
Operator : CG/JU
Sample : 02488-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039653.D
Acq On : 25 Apr 2023 23:17
Operator : CG/JU
Sample : 02488-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------