

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039654.D
 Acq On : 25 Apr 2023 23:53
 Operator : CG/JU
 Sample : 02488-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.172	19	23	26	rBV2	32895	45715	0.91%	0.102%
2	3.201	26	28	35	rVB	42089	53687	1.06%	0.120%
3	3.654	103	105	116	rBV	27000	63613	1.26%	0.142%
4	3.954	153	156	159	rBV2	13447	13993	0.28%	0.031%
5	4.401	228	232	235	rVB	14346	18272	0.36%	0.041%
6	4.490	242	247	252	rBV2	22040	34448	0.68%	0.077%
7	5.366	393	396	399	rVB2	8740	8937	0.18%	0.020%
8	5.495	414	418	422	rVB2	7519	11866	0.24%	0.026%
9	6.919	654	660	668	rBV	31122	46528	0.92%	0.104%
10	7.001	668	674	691	rBV2	119896	336848	6.67%	0.752%
11	7.142	692	698	720	rVV	736395	1296673	25.68%	2.896%
12	7.342	725	732	753	rBV	666816	1284009	25.43%	2.867%
13	7.807	805	811	827	rBV	637641	1143249	22.64%	2.553%
14	8.536	929	935	955	rBV	436773	994435	19.70%	2.221%
15	8.978	1004	1010	1030	rBV	786849	1526396	30.23%	3.409%
16	9.366	1072	1076	1080	rVB2	7994	12188	0.24%	0.027%
17	9.701	1127	1133	1148	rBV	668515	1269801	25.15%	2.836%
18	10.254	1220	1227	1255	rBV	556292	1664422	32.97%	3.717%
19	10.613	1281	1288	1307	rBV	997033	1729119	34.25%	3.861%
20	10.807	1314	1321	1339	rBV	18917	74444	1.47%	0.166%
21	11.860	1499	1500	1506	rVB6	3306	5232	0.10%	0.012%
22	12.236	1557	1564	1573	rBV5	10388	28090	0.56%	0.063%
23	13.277	1737	1741	1746	rVB6	4372	8084	0.16%	0.018%
24	13.360	1750	1755	1762	rVB7	8602	15727	0.31%	0.035%
25	13.883	1837	1844	1871	rBV	2162550	3322694	65.81%	7.420%
26	14.160	1884	1891	1910	rBV	1580527	2441536	48.36%	5.452%
27	14.360	1921	1925	1929	rVB6	3774	5686	0.11%	0.013%
28	14.465	1935	1943	1955	rBV	1350923	2061617	40.83%	4.604%
29	14.783	1990	1997	2002	rBV7	19229	59023	1.17%	0.132%
30	15.260	2075	2078	2082	rVB3	6040	8012	0.16%	0.018%
31	15.460	2106	2112	2130	rBV	2784267	4248101	84.14%	9.487%
32	15.601	2130	2136	2151	rBV	755517	1291539	25.58%	2.884%
33	15.836	2171	2176	2189	rVB	52285	96849	1.92%	0.216%
34	16.177	2230	2234	2238	rBV7	4455	7055	0.14%	0.016%
35	17.018	2372	2377	2382	rVB6	6759	11675	0.23%	0.026%
36	17.218	2405	2411	2422	rBV	1496778	2181727	43.21%	4.872%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039654.D
 Acq On : 25 Apr 2023 23:53
 Operator : CG/JU
 Sample : 02488-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

37	17.318	2422	2428	2446	rVV	2909865	4308069	85.33%	9.621%
38	17.889	2520	2525	2531	rBV9	10965	17398	0.34%	0.039%
39	18.118	2559	2564	2573	rBV	68419	138953	2.75%	0.310%
40	18.401	2609	2612	2617	rBV5	8374	11843	0.23%	0.026%
41	18.800	2678	2680	2683	rBV4	4910	5519	0.11%	0.012%
42	19.036	2718	2720	2726	rVB6	10004	11510	0.23%	0.026%
43	19.183	2741	2745	2752	rBV3	40892	59719	1.18%	0.133%
44	19.259	2754	2758	2761	rBV	33727	48777	0.97%	0.109%
45	19.400	2778	2782	2790	rBV6	41124	92720	1.84%	0.207%
46	19.542	2804	2806	2809	rVB2	16165	16206	0.32%	0.036%
47	19.618	2813	2819	2833	rBV	3624216	5048656	100.00%	11.275%
48	21.412	3120	3124	3140	rBV	1258163	1956549	38.75%	4.369%
49	23.624	3493	3500	3516	rVB2	1797068	3806288	75.39%	8.500%
50	23.771	3519	3525	3540	rVB2	803365	1835443	36.36%	4.099%




Sum of corrected areas: 44778940

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039654.D
Acq On : 25 Apr 2023 23:53
Operator : CG/JU
Sample : 02488-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

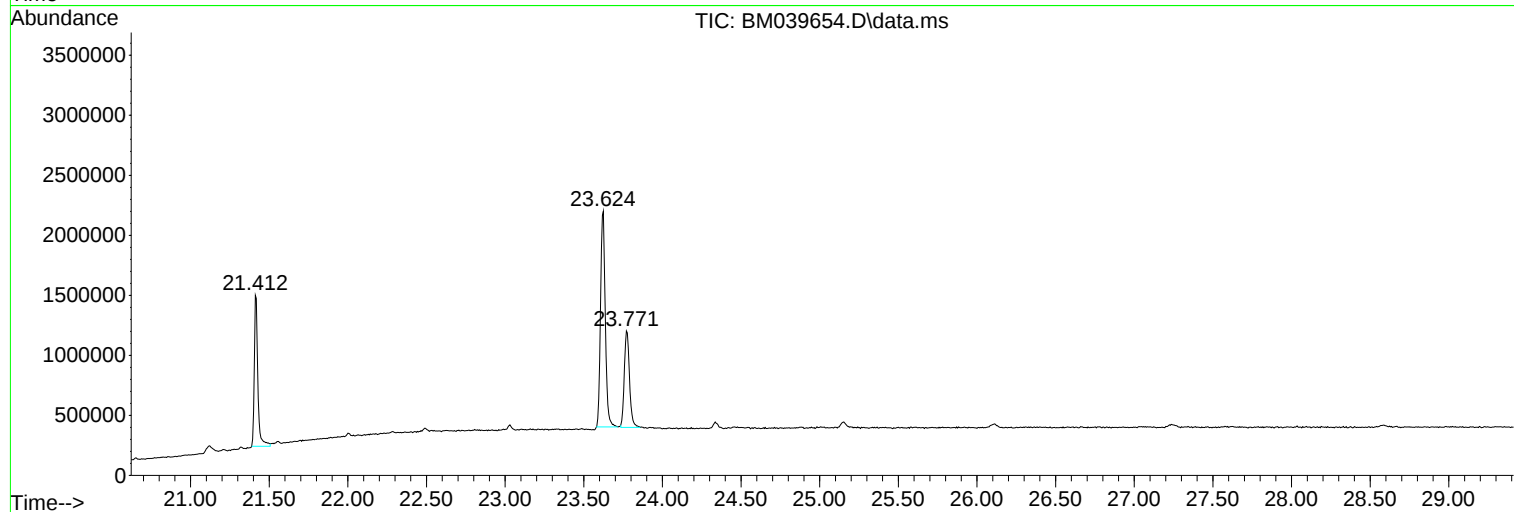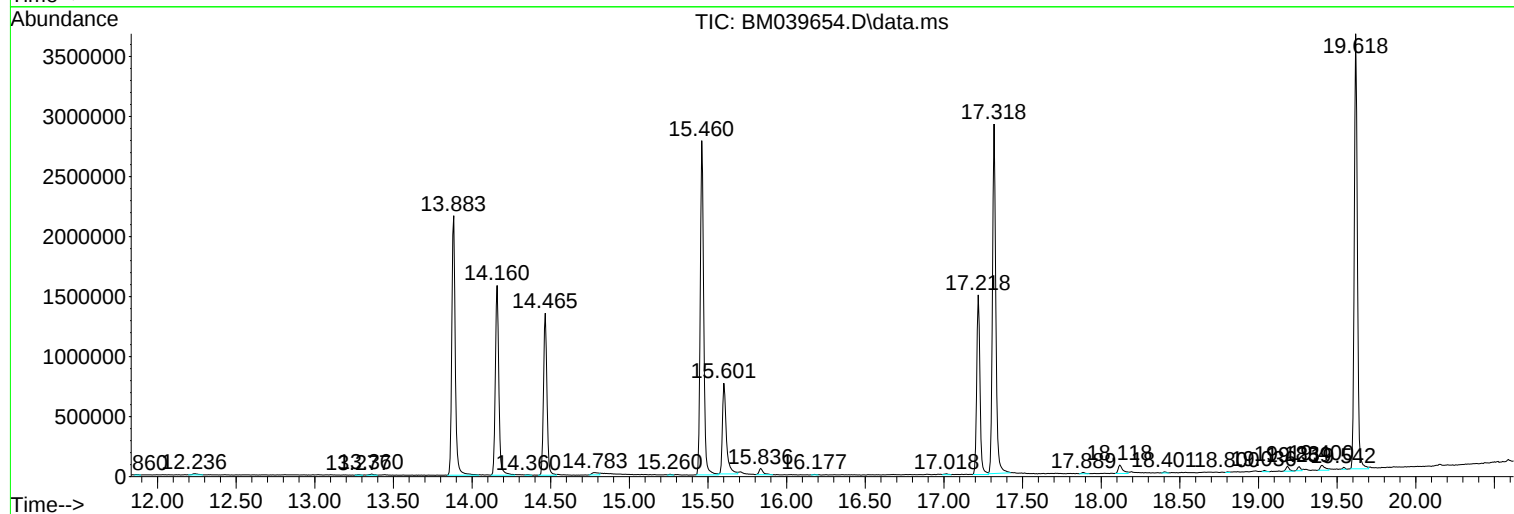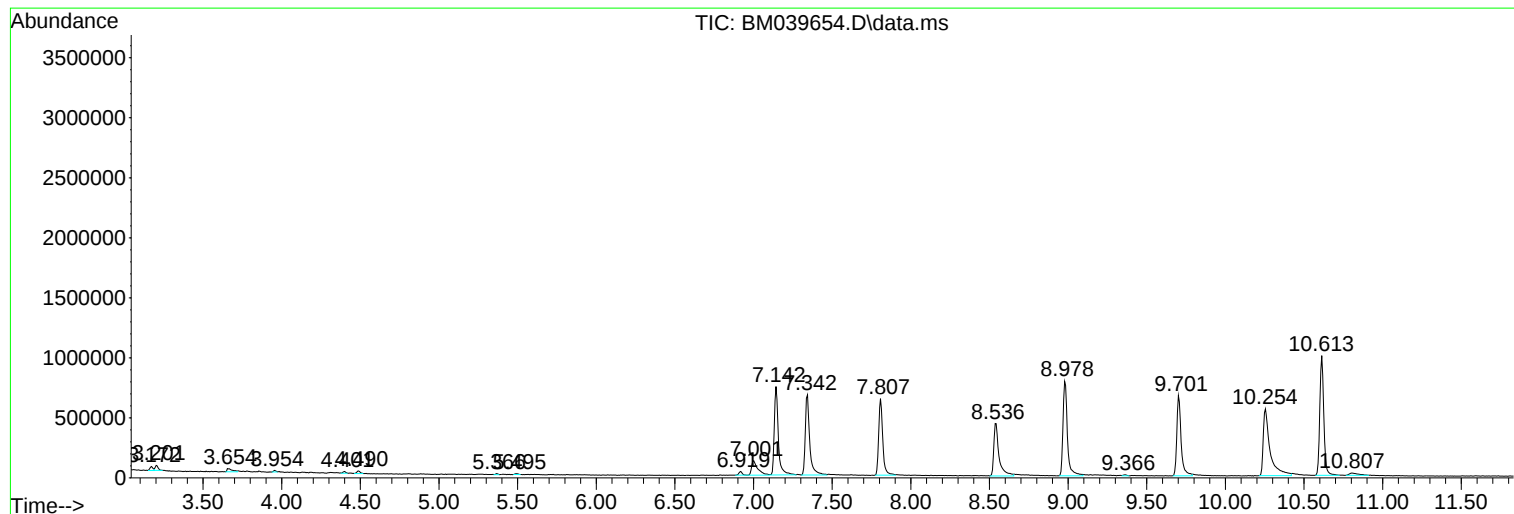

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039654.D
Acq On : 25 Apr 2023 23:53
Operator : CG/JU
Sample : 02488-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039654.D
Acq On : 25 Apr 2023 23:53
Operator : CG/JU
Sample : 02488-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc