

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
 Data File : BM039657.D
 Acq On : 26 Apr 2023 01:42
 Operator : CG/JU
 Sample : PB152238BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK238

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.078	5	7	10	rVB	37449	35081	1.26%	0.261%
2	3.119	10	14	22	rVB	570227	575084	20.64%	4.286%
3	3.460	69	72	78	rVB2	19591	22929	0.82%	0.171%
4	3.954	151	156	161	rBV	17038	25633	0.92%	0.191%
5	5.896	482	486	487	rVV4	2556	2972	0.11%	0.022%
6	6.925	659	661	664	rVB4	3923	4695	0.17%	0.035%
7	7.807	804	811	835	rBV	677330	1364274	48.95%	10.168%
8	8.042	849	851	856	rVB6	2413	3541	0.13%	0.026%
9	8.707	960	964	966	rBV5	2063	3265	0.12%	0.024%
10	8.954	1001	1006	1008	rBV5	2635	3881	0.14%	0.029%
11	9.048	1019	1022	1026	rBV6	2050	3552	0.13%	0.026%
12	9.495	1094	1098	1099	rBV3	3476	3107	0.11%	0.023%
13	10.613	1280	1288	1313	rBV	999252	2038037	73.13%	15.189%
14	14.466	1936	1943	1962	rBV	1578837	2601232	93.34%	19.387%
15	15.189	2064	2066	2071	rBV6	1804	2791	0.10%	0.021%
16	17.012	2373	2376	2377	rBV3	2962	3179	0.11%	0.024%
17	17.218	2405	2411	2430	rBV	1470259	2786837	100.00%	20.770%
18	17.571	2470	2471	2475	rBV4	2345	3635	0.13%	0.027%
19	17.736	2497	2499	2503	rBV4	2184	3183	0.11%	0.024%
20	21.412	3119	3124	3140	rBV	1397615	2267458	81.36%	16.899%
21	23.777	3520	3526	3539	rVB2	733533	1663318	59.68%	12.396%




Sum of corrected areas: 13417684

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039657.D
Acq On : 26 Apr 2023 01:42
Operator : CG/JU
Sample : PB152238BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK238

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

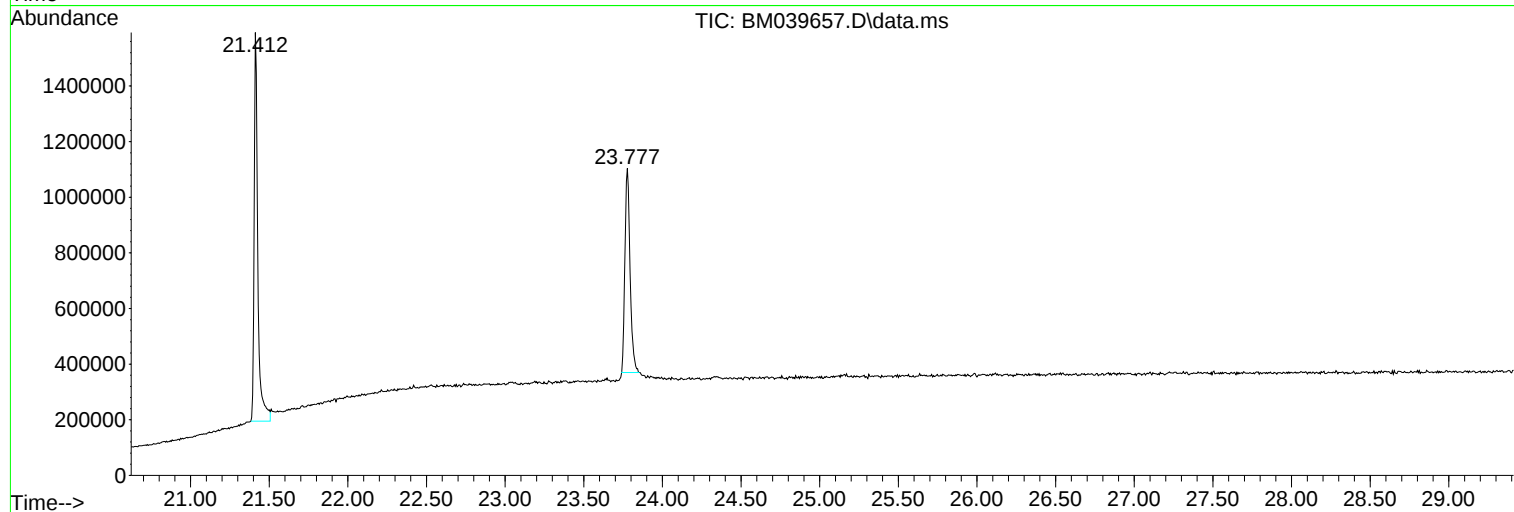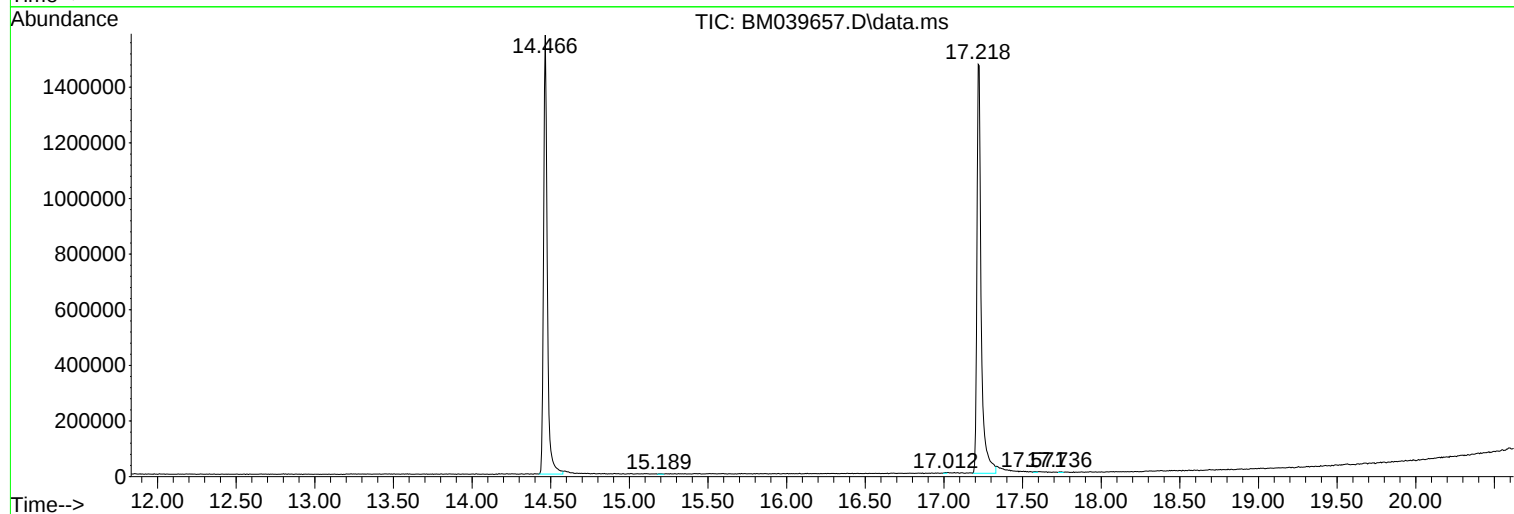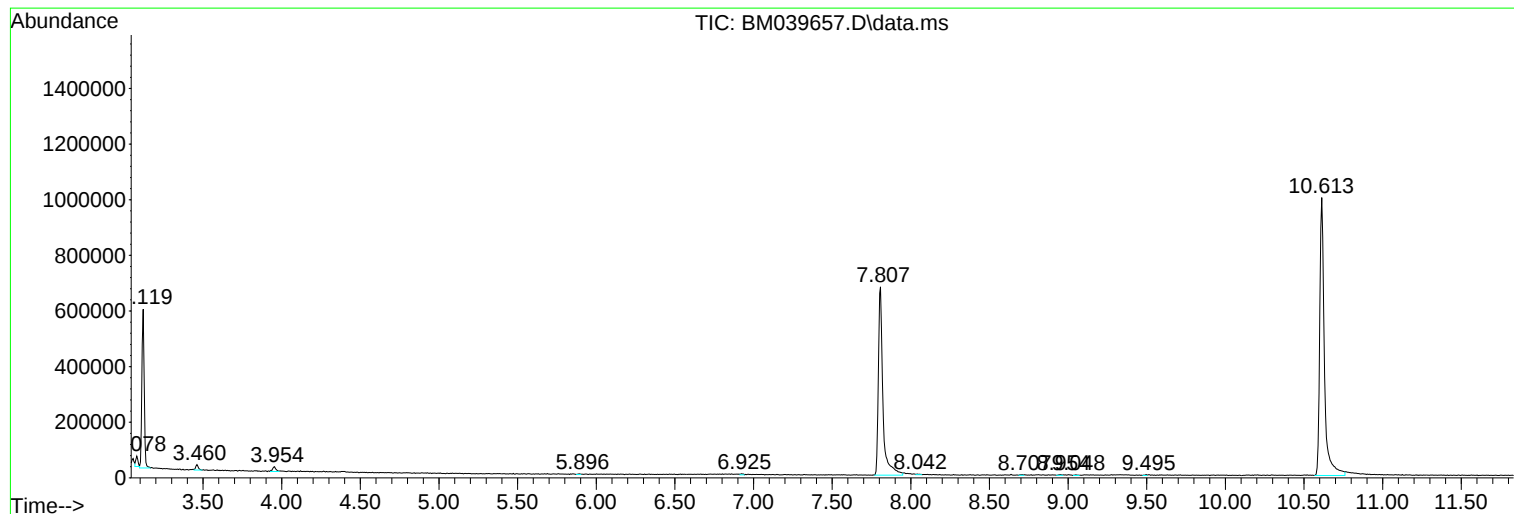

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039657.D
Acq On : 26 Apr 2023 01:42
Operator : CG/JU
Sample : PB152238BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK238










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.119	8.43 ng/ul	575084	1,4-Dichlorobenzene-d4	7.807

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	94
2			Heptane	100	C7H16	000142-82-5	94
3			Heptane	100	C7H16	000142-82-5	91
4			Heptane	100	C7H16	000142-82-5	83
5			Oxalic acid, isobutyl pentyl ester	216	C11H20O4	1000309-37-0	64

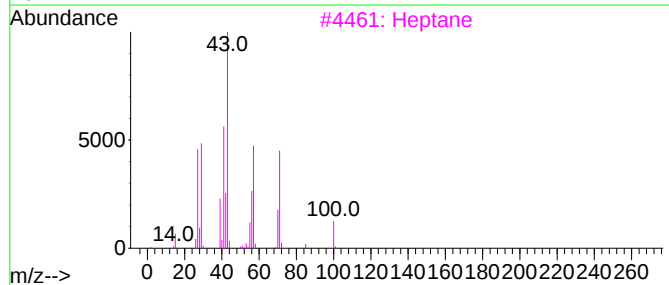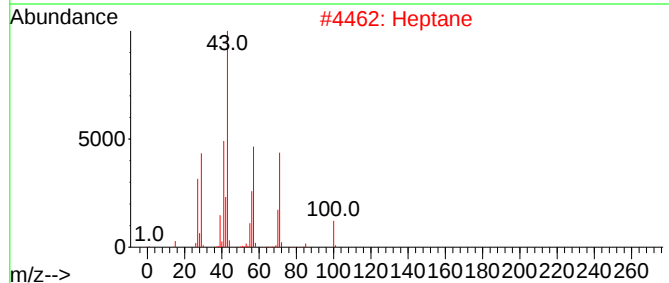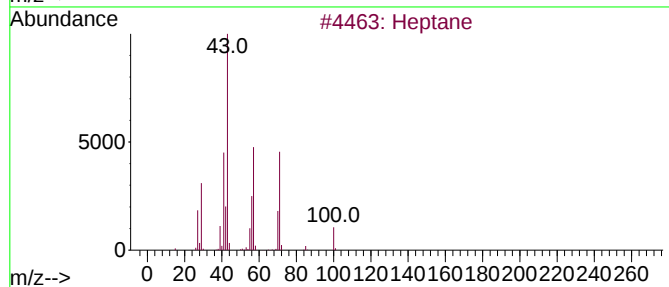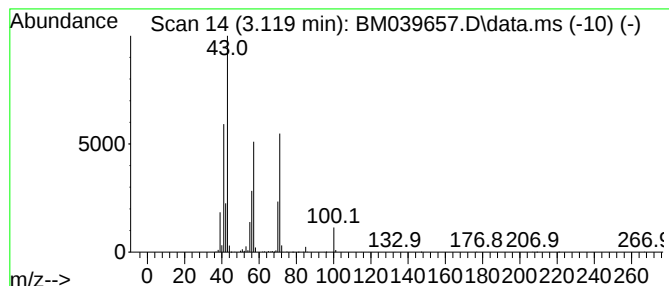

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042523\
Data File : BM039657.D
Acq On : 26 Apr 2023 01:42
Operator : CG/JU
Sample : PB152238BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK238

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.119	8.4	ng/u1	575084	1	7.807	1364270	20.0