


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042524\
Data File : BM045565.D
Acq On : 25 Apr 2024 16:00
Operator : MA/JU
Sample : DFTPP019
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP019

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM042024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Apr 24 05:17:39 2024

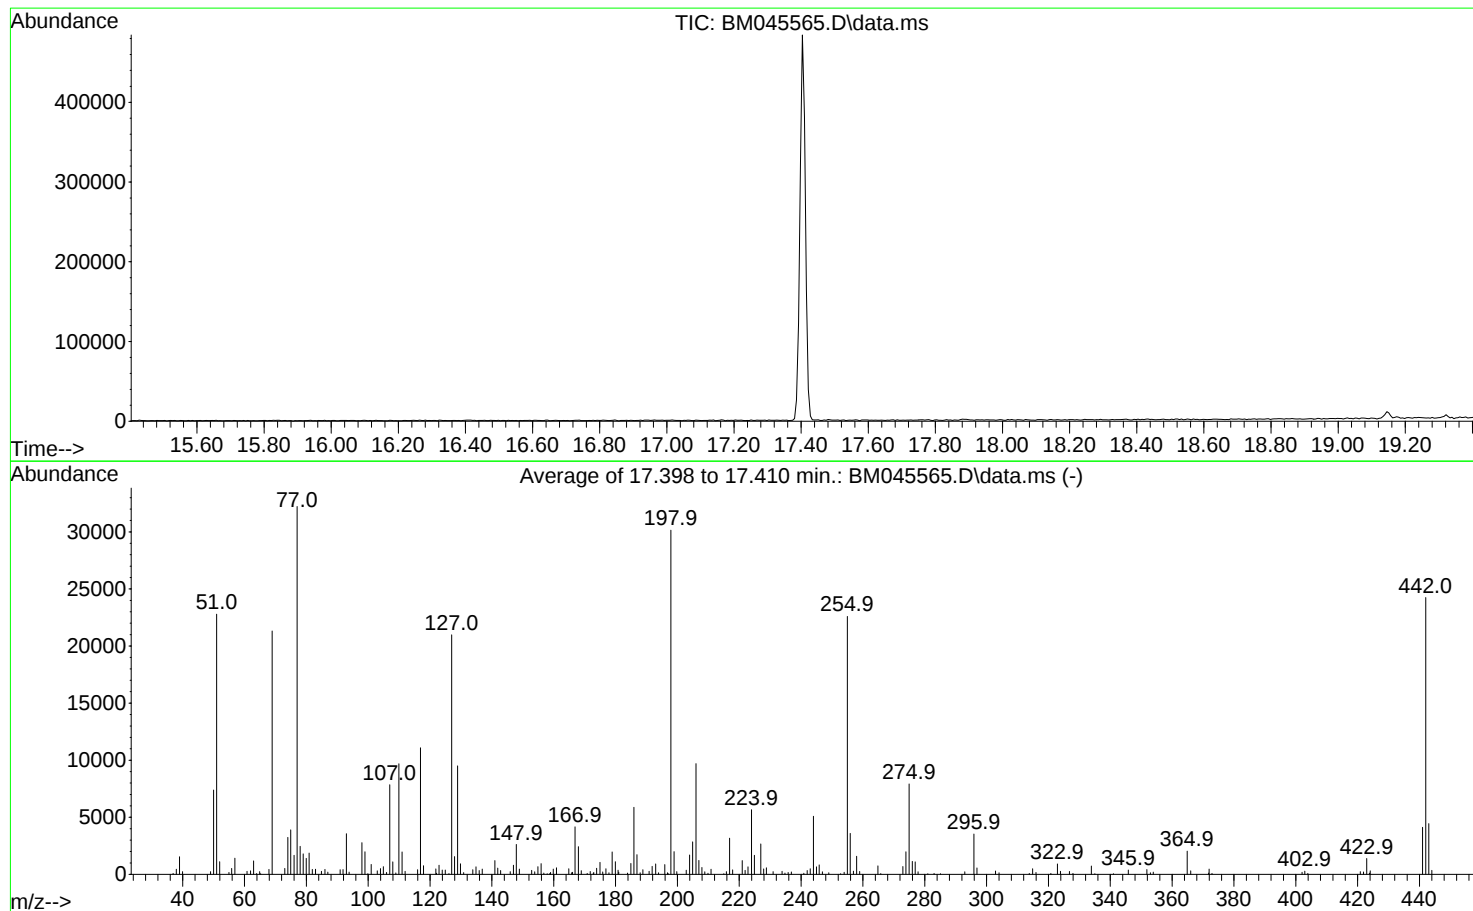

AutoFind: Scans 2433, 2434, 2435; Background Corrected with Scan 2427

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	75.6	22789	PASS
68	69	0.00	2	2.0	432	PASS
69	198	0.00	100	70.7	21312	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	69.6	20987	PASS
197	198	0.00	2	0.5	137	PASS
198	198	100	100	100.0	30152	PASS
199	198	5	9	6.6	1988	PASS
275	198	10	60	26.3	7922	PASS
365	198	1	100	6.8	2037	PASS
441	198	0.01	100	13.7	4128	PASS
442	198	50	100	80.4	24244	PASS
443	442	15	24	18.3	4448	PASS

Scan 2427 (17.363 min): BM045565.D\data.ms
DFTPP019

m/z	Abundance
44.00	312.0
207.00	560.0

Instrument :

BNA_M

ClientSampleId :

DFTPP019

m/z	Abundance
38.00	390.0
39.00	1503.0
40.00	204.0
44.00	382.0
49.00	259.0
50.00	7227.0
51.00	20440.0
52.00	989.0
55.80	606.0
56.90	1488.0
60.80	318.0
62.00	313.0
62.90	1155.0
64.90	273.0
67.90	362.0
68.90	19832.0
73.00	507.0
74.00	2840.0
75.00	3932.0
76.00	1432.0
77.00	30512.0
78.00	2545.0
79.00	1451.0
79.90	1114.0
80.90	1704.0
81.90	319.0
83.00	433.0
84.80	299.0
86.00	481.0
87.10	201.0
91.00	437.0
91.80	394.0
92.90	3120.0
94.00	188.0
98.00	2617.0
98.90	1739.0
99.90	165.0
101.00	826.0
102.90	246.0
104.00	553.0
104.90	562.0
105.90	196.0
106.90	7165.0
108.00	884.0
109.00	170.0
109.90	9119.0
111.00	1538.0
112.00	265.0
116.00	323.0
116.90	9270.0
117.90	576.0
121.80	306.0
122.10	305.0
122.90	598.0
124.00	337.0
124.90	201.0
127.00	18000.0
127.90	1282.0
128.90	8132.0
129.90	921.0
130.90	207.0
133.90	289.0
134.90	478.0
135.90	256.0
136.90	416.0
140.90	960.0
142.00	504.0
142.80	294.0
145.90	178.0
146.90	707.0
147.90	2157.0
149.00	597.0
152.80	248.0
153.80	173.0
154.90	588.0
155.90	779.0
158.90	304.0
159.90	318.0
160.90	505.0
164.80	278.0
166.10	220.0
166.90	3550.0
168.00	1994.0
168.90	201.0
170.80	241.0
171.70	198.0
172.80	238.0
173.90	368.0
174.90	861.0
176.90	292.0
178.90	1597.0
180.00	973.0

Instrument :
BNA_M
ClientSampleId :
DFTPP019

180.80	397.0
183.90	181.0
184.90	743.0
186.00	4880.0
186.90	1422.0
187.90	246.0
188.80	371.0
190.90	283.0
191.90	520.0
192.90	613.0
193.90	202.0
195.90	681.0
196.80	204.0
197.90	23344.0
198.90	1286.0
199.80	245.0
202.90	427.0
203.90	1091.0
204.90	2004.0
206.00	8163.0
207.00	1255.0
207.90	547.0
208.90	194.0
210.90	358.0
215.90	277.0
216.90	2470.0
217.80	415.0
221.00	1066.0
222.80	536.0
224.00	3835.0
224.90	1350.0
226.90	2088.0
227.90	387.0
228.80	660.0
231.00	207.0
233.90	209.0
234.80	151.0
236.80	217.0
240.90	279.0
242.00	292.0
243.00	520.0
244.00	3851.0
245.10	486.0
245.90	565.0
247.00	190.0
253.90	155.0
254.90	16920.0
255.90	2507.0
256.90	247.0
258.00	1254.0
258.90	223.0
264.90	702.0
272.90	493.0
273.90	1551.0
274.90	5557.0
275.90	950.0
276.90	683.0
277.90	195.0
292.90	196.0
295.90	2465.0
296.90	602.0
314.90	390.0
322.90	770.0
323.90	229.0
326.80	162.0
333.90	613.0
345.90	182.0
351.90	182.0
364.90	1341.0
366.00	251.0
371.80	322.0
402.80	163.0
420.90	234.0
422.00	173.0
422.90	563.0
423.80	319.0
441.00	2431.0
442.00	14196.0
443.00	2487.0
444.00	212.0

Instrument :
BNA_M
ClientSampleId :
DFTPP019

m/z	Abundance
36.90	253.0
37.90	617.0
39.00	1853.0
39.90	237.0
43.90	342.0
49.00	302.0
50.00	9021.0
51.00	28168.0
52.00	1267.0
55.00	274.0
55.90	592.0
56.90	1750.0
60.80	307.0
61.90	365.0
62.90	1327.0
63.90	221.0
64.90	449.0
67.90	575.0
69.00	26040.0
73.10	512.0
74.00	3958.0
75.00	4279.0
76.00	2060.0
77.00	40072.0
78.00	2863.0
79.00	2137.0
80.00	1916.0
80.90	2094.0
81.90	651.0
82.90	371.0
84.90	273.0
86.00	476.0
86.90	381.0
90.90	505.0
91.90	528.0
92.90	4513.0
93.80	411.0
97.90	3414.0
98.90	2680.0
100.90	1080.0
103.00	452.0
103.90	586.0
104.90	816.0
106.00	308.0
107.00	9408.0
107.90	1551.0
108.90	195.0
109.90	11423.0
111.00	2590.0
112.00	337.0
115.90	503.0
116.90	13499.0
117.90	1115.0
121.90	586.0
122.90	1065.0
124.00	508.0
125.00	466.0
126.10	198.0
127.00	25240.0
128.00	1984.0
128.90	12229.0
129.90	1019.0
130.90	267.0
133.80	502.0
134.90	961.0
135.90	556.0
136.90	642.0
141.00	1312.0
141.80	585.0
142.90	325.0
145.90	323.0
146.90	1007.0
147.90	3237.0
148.80	469.0
152.90	602.0
153.90	287.0
154.90	878.0
155.90	1159.0
157.90	181.0
159.00	181.0
159.80	486.0
160.80	550.0
164.90	458.0
165.80	442.0
166.90	4968.0
168.00	3164.0
168.90	510.0
171.80	363.0
173.00	277.0
173.90	640.0
175.00	1374.0
175.80	334.0

Instrument :
BNA_M
ClientSampleId :
DFTPP019

176.90	698.0
177.80	211.0
178.90	2489.0
179.90	1281.0
180.80	692.0
183.80	171.0
184.90	1316.0
185.90	6959.0
186.90	1910.0
188.00	172.0
188.90	532.0
190.80	249.0
191.90	980.0
193.00	1018.0
193.90	236.0
195.90	1059.0
197.00	221.0
197.90	36440.0
198.90	2485.0
199.80	232.0
202.90	370.0
204.00	2172.0
205.00	3693.0
206.00	11853.0
206.90	1972.0
208.00	731.0
208.90	200.0
209.90	303.0
210.80	489.0
215.00	165.0
215.80	285.0
216.90	3661.0
217.80	411.0
220.90	1552.0
222.00	489.0
222.90	826.0
223.90	7289.0
224.90	1970.0
226.90	3028.0
227.90	682.0
228.80	565.0
231.00	317.0
233.90	253.0
234.80	171.0
235.80	335.0
236.80	232.0
242.00	290.0
242.90	499.0
244.00	6033.0
244.90	731.0
245.90	1241.0
246.90	236.0
249.00	171.0
254.00	228.0
255.00	27944.0
255.90	4329.0
257.00	325.0
258.00	1800.0
258.90	244.0
264.90	843.0
265.80	221.0
272.90	839.0
273.90	2312.0
275.00	9433.0
276.00	1394.0
276.90	1386.0
277.70	295.0
292.90	261.0
295.90	4095.0
296.90	763.0
302.90	383.0
304.10	184.0
313.80	243.0
314.90	483.0
316.00	228.0
320.80	237.0
322.90	1072.0
323.90	301.0
326.70	345.0
327.90	248.0
333.90	729.0
345.80	408.0
351.90	638.0
352.90	189.0
353.90	393.0
364.90	2562.0
366.00	318.0
372.00	597.0
372.90	263.0
402.00	331.0
402.90	363.0
403.90	235.0
420.80	241.0
421.90	181.0
422.90	1802.0
424.00	499.0

Instrument :
BNA_M
ClientSampleId :
DFTPP019

441.00	4960.0
442.00	28808.0
443.00	5175.0
444.00	323.0

Instrument :
BNA_M
ClientSampleId :
DFTPP019

m/z	Abundance
38.00	345.0
39.00	1267.0
39.90	262.0
43.80	205.0
49.00	152.0
50.00	5891.0
51.00	19760.0
51.90	1049.0
54.90	215.0
55.90	377.0
56.90	1008.0
60.90	187.0
61.90	259.0
63.00	1041.0
65.20	181.0
67.90	358.0
69.00	18064.0
73.00	543.0
74.00	2933.0
74.90	3476.0
76.00	1533.0
77.00	26088.0
78.00	1973.0
79.00	1783.0
79.90	1195.0
80.90	1784.0
81.90	335.0
83.00	522.0
84.90	240.0
86.00	365.0
91.00	273.0
91.90	355.0
93.00	3067.0
97.90	2302.0
99.00	1501.0
100.90	712.0
102.90	248.0
103.90	393.0
104.90	658.0
107.00	6959.0
108.00	856.0
109.90	8534.0
110.90	1770.0
111.90	208.0
116.00	391.0
116.90	10483.0
117.90	600.0
121.80	524.0
122.90	729.0
123.90	302.0
124.90	448.0
127.00	19720.0
128.00	1413.0
128.90	8148.0
129.80	839.0
133.90	429.0
134.80	557.0
135.90	197.0
136.90	335.0
140.90	1334.0
141.90	575.0
142.80	401.0
146.00	197.0
147.00	686.0
147.90	2456.0
148.90	340.0
152.80	218.0
153.90	232.0
154.90	554.0
155.90	866.0
156.80	321.0
158.70	191.0
159.90	601.0
161.00	666.0
164.90	719.0
166.00	309.0
166.90	3981.0
168.00	2133.0
168.90	254.0
171.90	206.0
172.90	241.0
173.90	612.0
174.90	936.0
175.90	285.0
176.90	502.0
177.90	228.0
178.90	1810.0
179.90	1082.0
181.00	580.0
185.00	809.0
186.00	5800.0
186.90	1859.0

Instrument :
BNA_M
ClientSampleId :
DFTPP019

188.90	307.0
190.80	268.0
191.80	595.0
192.90	1108.0
195.90	840.0
196.80	206.0
197.90	30672.0
198.90	2193.0
199.80	252.0
202.80	317.0
203.90	1846.0
205.00	2834.0
206.00	9084.0
207.00	2094.0
208.00	515.0
208.80	277.0
210.80	492.0
215.80	162.0
216.90	3361.0
217.90	332.0
220.90	1000.0
221.80	575.0
222.90	604.0
224.00	5850.0
224.90	1670.0
227.00	2886.0
227.90	365.0
228.80	516.0
230.90	212.0
233.80	337.0
235.80	158.0
236.90	199.0
241.90	442.0
242.90	437.0
244.00	5379.0
245.00	780.0
245.80	690.0
246.80	263.0
248.90	236.0
252.80	187.0
254.00	157.0
255.00	22936.0
255.90	3936.0
256.90	265.0
257.90	1682.0
259.00	272.0
264.80	668.0
272.90	748.0
273.90	2087.0
275.00	8777.0
276.00	1048.0
276.90	1196.0
277.90	173.0
281.00	189.0
283.00	273.0
285.10	177.0
293.00	237.0
295.90	4042.0
296.90	310.0
302.90	508.0
303.90	237.0
314.90	596.0
315.90	257.0
322.90	876.0
323.90	288.0
326.90	236.0
333.90	865.0
335.00	158.0
341.00	166.0
345.90	529.0
351.80	421.0
353.00	252.0
353.90	210.0
364.80	2208.0
366.00	364.0
371.90	805.0
402.00	222.0
403.00	298.0
420.80	243.0
421.80	267.0
423.00	1791.0
424.10	433.0
441.00	4994.0
442.00	29728.0
443.00	5683.0
444.00	516.0

Instrument :
BNA_M
ClientSampleId :
DFTPP019