

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042617\
 Data File : BM009727.D
 Acq On : 26 Apr 2017 19:24
 Operator : SJ/MA
 Sample : I2836-13
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 27 00:53:42 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 27 00:53:43 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	170257	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	757248	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	486173	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1168593	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1444787	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	1110600	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	13984	3.78	ng/uL	0.00
5) Phenol-d5	6.99	99	352116	19.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	254696	20.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	240868	20.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	290483	20.15	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	130126	21.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	138465	21.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	265471	20.47	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	331907	21.24	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	900897	21.30	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1102216	21.61	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	146430	17.94	ng/ul	0.00
57) Fluorene-d10	15.47	176	849219	22.25	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	135340	16.42	ng/ul	0.00
70) Anthracene-d10	17.32	188	1384113	23.07	ng/ul	0.00
76) Pyrene-d10	19.62	212	1677718	26.31	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1327147	24.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.93	163	185386	4.43	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042617\
Data File : BM009727.D
Acq On : 26 Apr 2017 19:24
Operator : SJ/MA
Sample : I2836-13
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :

Quant Time: Apr 27 00:53:42 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 27 00:53:43 2017
Response via : Initial Calibration

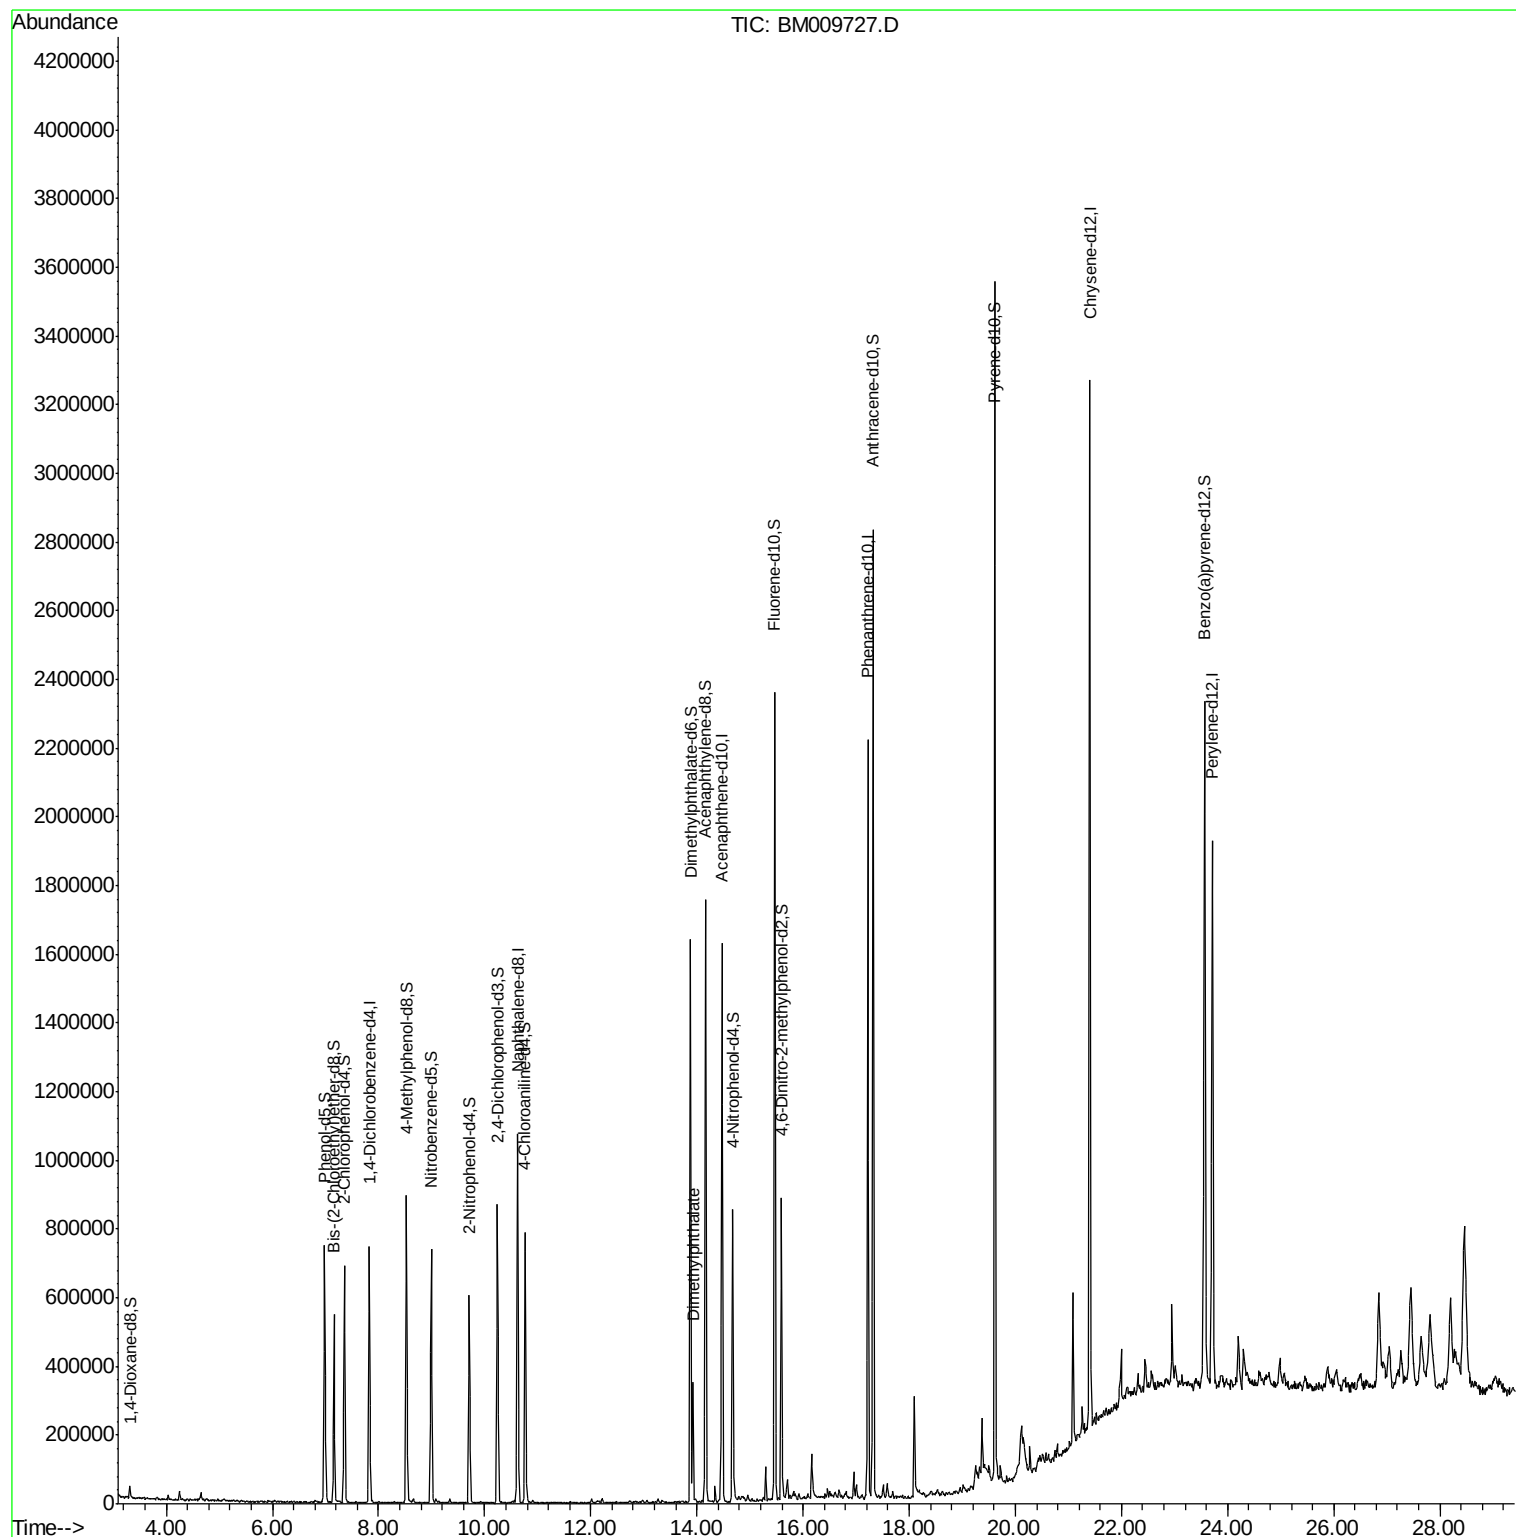


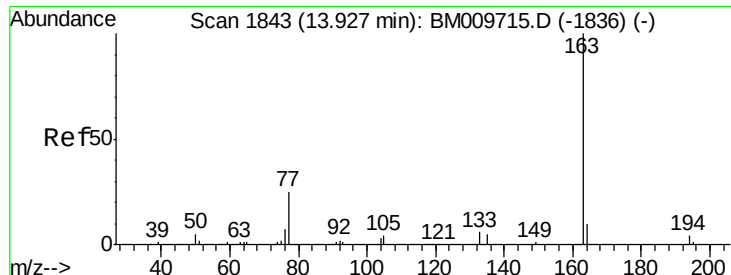

#44
 Dimethylphthalate
 Concen: 4.43 ng/ul
 RT: 13.93 min Scan# 1843
 Delta R.T. -0.00 min
 Lab File: BM009727.D
 Acq: 26 Apr 2017 19:24

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:	163	Resp:	185386
Ion Ratio	Lower	Upper	
163	100		
194	4.3	3.0	4.6
164	9.2	8.6	12.8

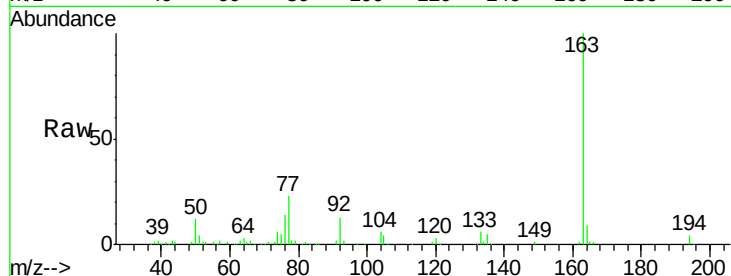

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

