

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042617\
 Data File : BM009728.D
 Acq On : 26 Apr 2017 20:00
 Operator : SJ/MA
 Sample : I2836-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 27 00:53:52 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 27 00:53:43 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	179254	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	782305	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	502837	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1176999	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1185083	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	930284	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	15207	3.91	ng/uL	0.00
5) Phenol-d5	6.99	99	346513	17.79	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	254788	19.19	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	240896	19.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	281437	18.54	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	126287	19.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	135166	20.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	263457	19.66	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	328971	20.38	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	910250	20.81	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1088970	20.64	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	145461	17.24	ng/ul	0.00
57) Fluorene-d10	15.47	176	817864	20.71	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	141156	17.00	ng/ul	0.00
70) Anthracene-d10	17.32	188	1313839	21.74	ng/ul	0.00
76) Pyrene-d10	19.62	212	1431563	27.37	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	999433	22.09	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.93	163	171478	3.96	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042617\
Data File : BM009728.D
Acq On : 26 Apr 2017 20:00
Operator : SJ/MA
Sample : I2836-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :

Quant Time: Apr 27 00:53:52 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 27 00:53:43 2017
Response via : Initial Calibration

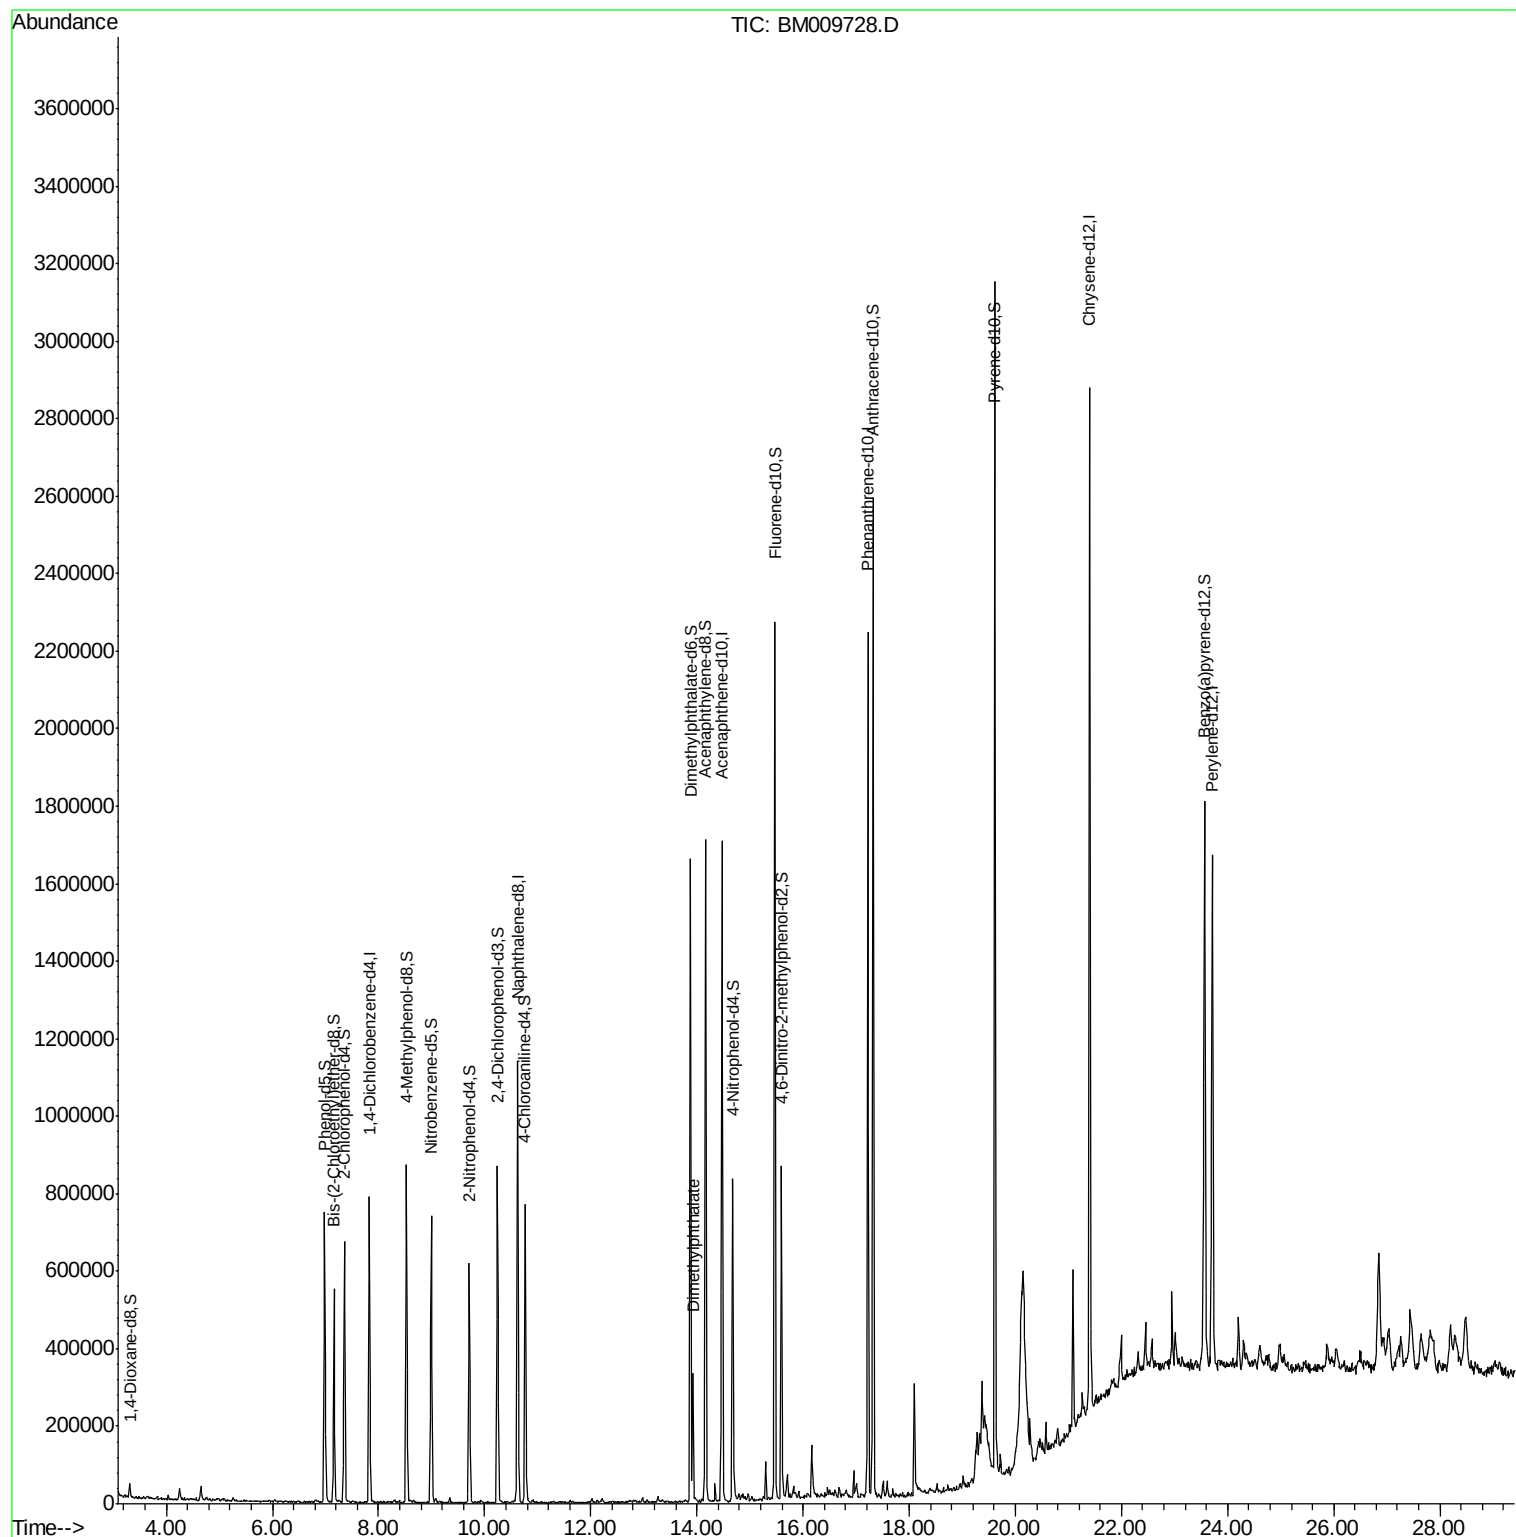


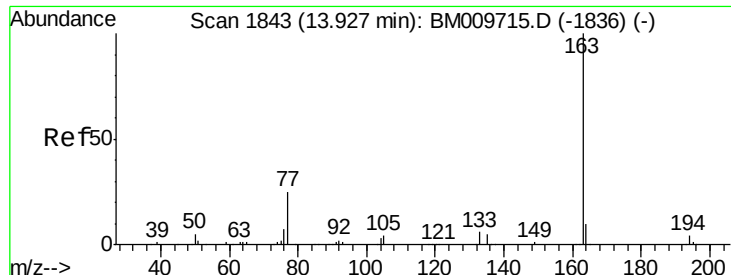

#44
 Dimethylphthalate
 Concen: 3.96 ng/ul
 RT: 13.93 min Scan# 1843
 Delta R.T. -0.00 min
 Lab File: BM009728.D
 Acq: 26 Apr 2017 20:00

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.0	4.6
164	8.4	8.6	12.8#

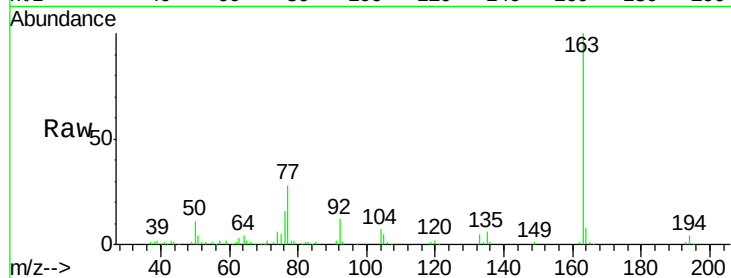

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

