

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042617\
 Data File : BM009717.D
 Acq On : 26 Apr 2017 13:24
 Operator : SJ/MA
 Sample : I2836-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CEM-BF001-01

Quant Time: Apr 26 16:11:44 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Apr 26 16:06:51 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	105016	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	438376	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	279249	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	692613	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1075746	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	1126938	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	7009	3.07	ng/uL	0.00
5) Phenol-d5	6.99	99	153503	13.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	117713	15.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	106860	14.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	109474	12.31	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	55530	15.56	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	57638	15.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	100528	13.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	120463	13.32	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	392311	16.15	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	457049	15.60	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	56294	12.01	ng/ul	0.00
57) Fluorene-d10	15.46	176	354055	16.15	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	55024	11.26	ng/ul	0.00
70) Anthracene-d10	17.32	188	582592	16.38	ng/ul	0.00
76) Pyrene-d10	19.62	212	763049	16.07	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	926391	16.90	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.92	163	75660	3.15	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042617\
Data File : BM009717.D
Acq On : 26 Apr 2017 13:24
Operator : SJ/MA
Sample : I2836-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CEM-BF001-01

Quant Time: Apr 26 16:11:44 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Apr 26 16:06:51 2017
Response via : Initial Calibration

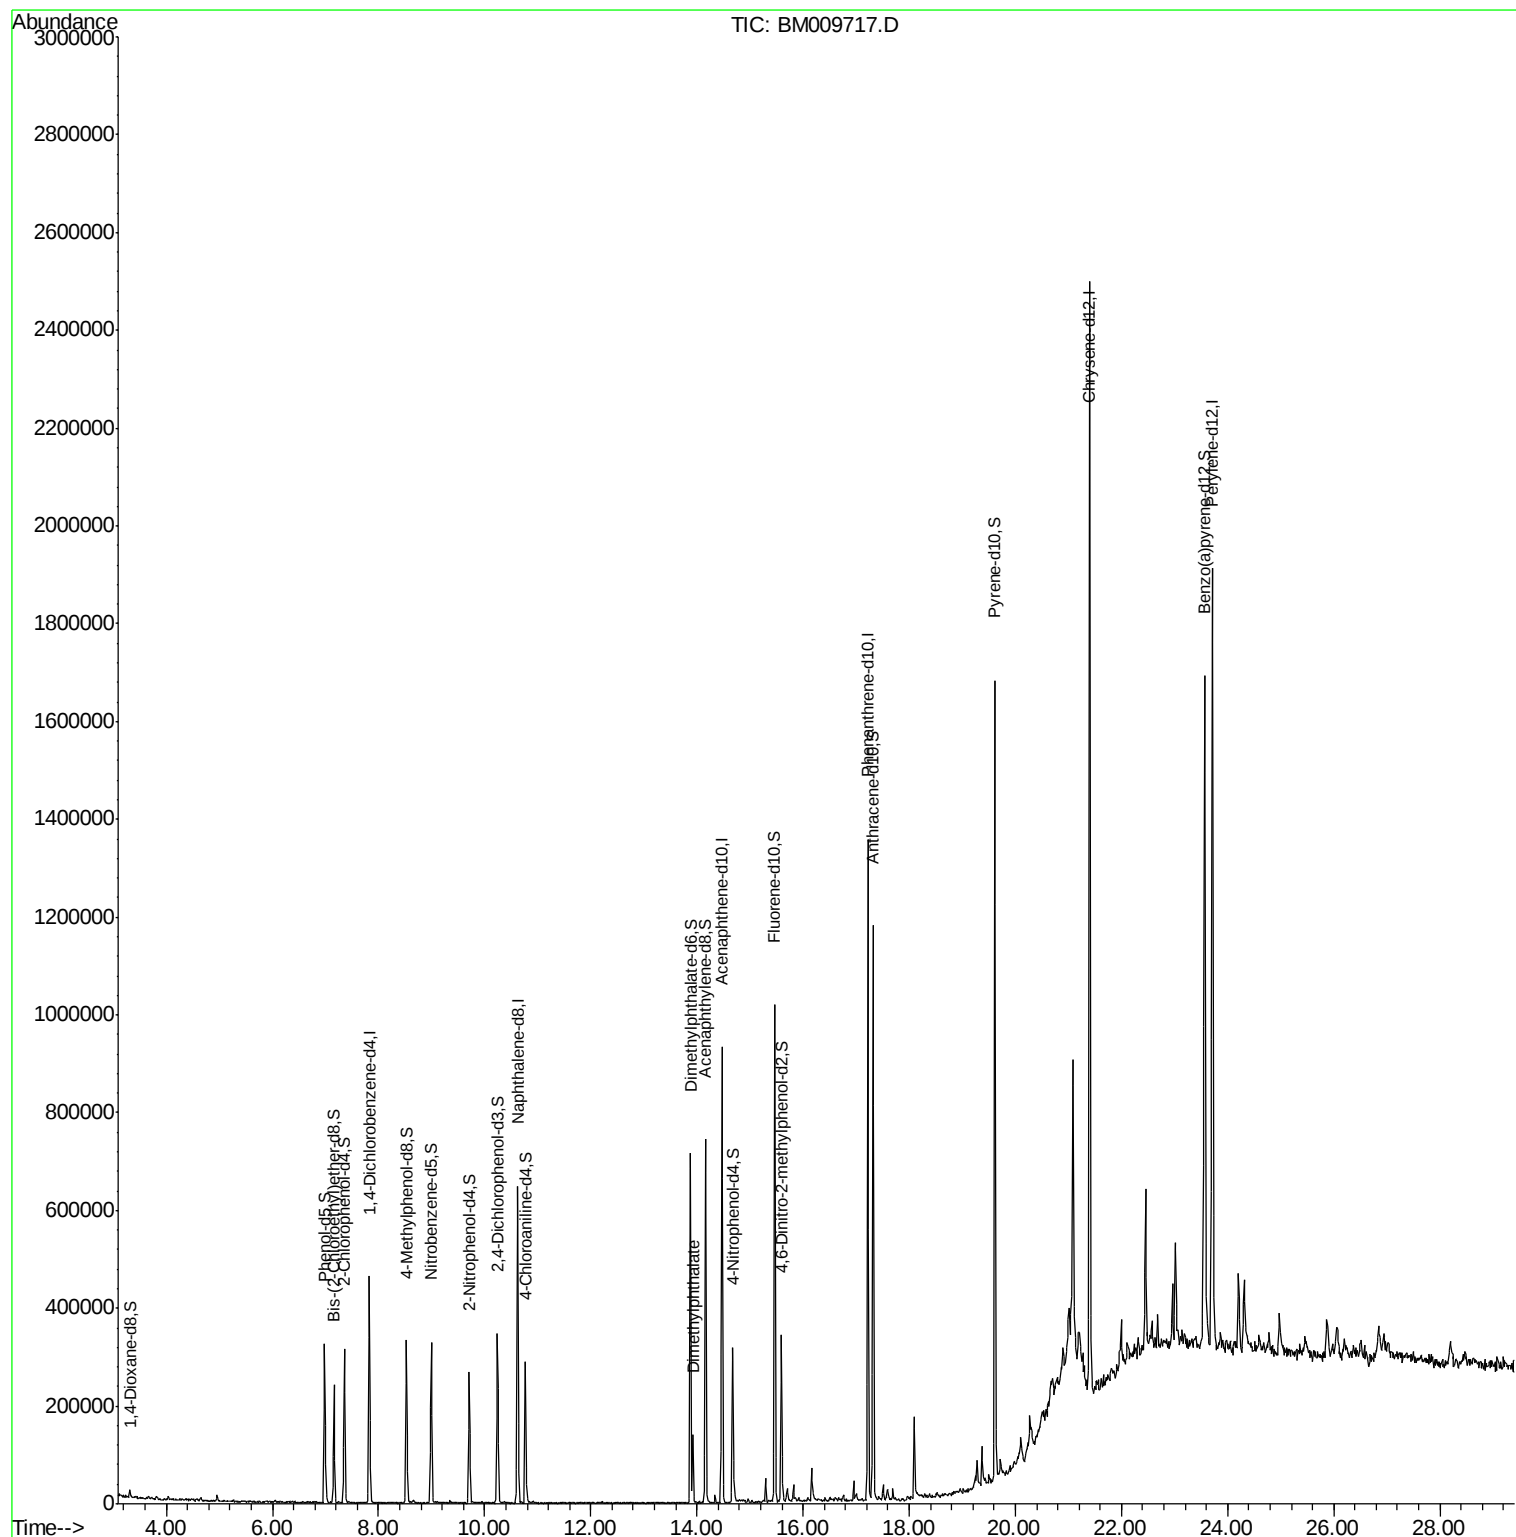


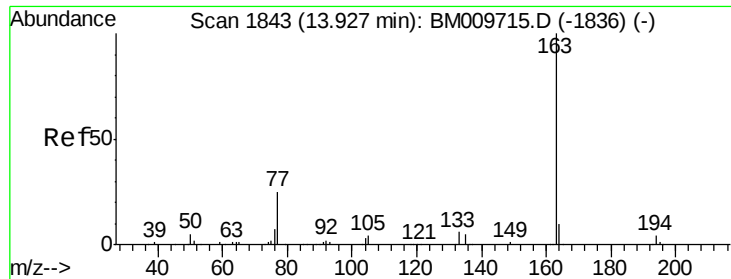

#44
 Dimethylphthalate
 Concen: 3.15 ng/ul
 RT: 13.92 min Scan# 1842
 Delta R.T. -0.01 min
 Lab File: BM009717.D
 Acq: 26 Apr 2017 13:24

Instrument :
 BNA_M
 ClientSampleId :
 CEM-BF001-01

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.0	4.6
164	8.9	8.6	12.8

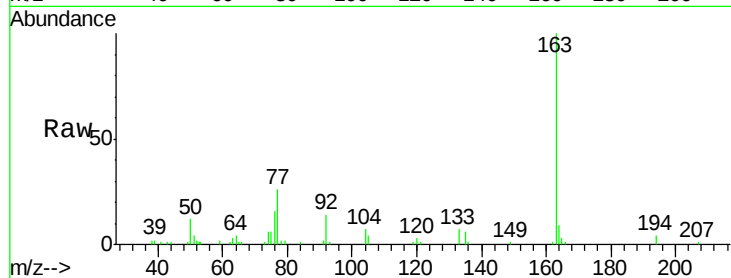

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

