

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042617\
 Data File : BM009724.D
 Acq On : 26 Apr 2017 17:36
 Operator : SJ/MA
 Sample : I2836-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EME-TS001-01

Quant Time: Apr 26 18:15:26 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 13:32:43 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	148657	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	643333	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	398615	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	994510	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1237319	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	970526	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	10681	3.31	ng/uL	0.00
5) Phenol-d5	6.99	99	266857	16.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	198676	18.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	187187	18.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	215161	17.09	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	97818	18.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	100747	18.29	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	194305	17.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	246570	18.57	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	703342	20.28	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	821039	19.63	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	114989	17.19	ng/ul	0.00
57) Fluorene-d10	15.47	176	639248	20.42	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	110361	15.73	ng/ul	0.00
70) Anthracene-d10	17.32	188	1081524	21.18	ng/ul	0.00
76) Pyrene-d10	19.62	212	1297077	23.75	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1022513	21.66	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.93	163	125628	3.66	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042617\
Data File : BM009724.D
Acq On : 26 Apr 2017 17:36
Operator : SJ/MA
Sample : I2836-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EME-TS001-01

Quant Time: Apr 26 18:15:26 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 25 13:32:43 2017
Response via : Initial Calibration

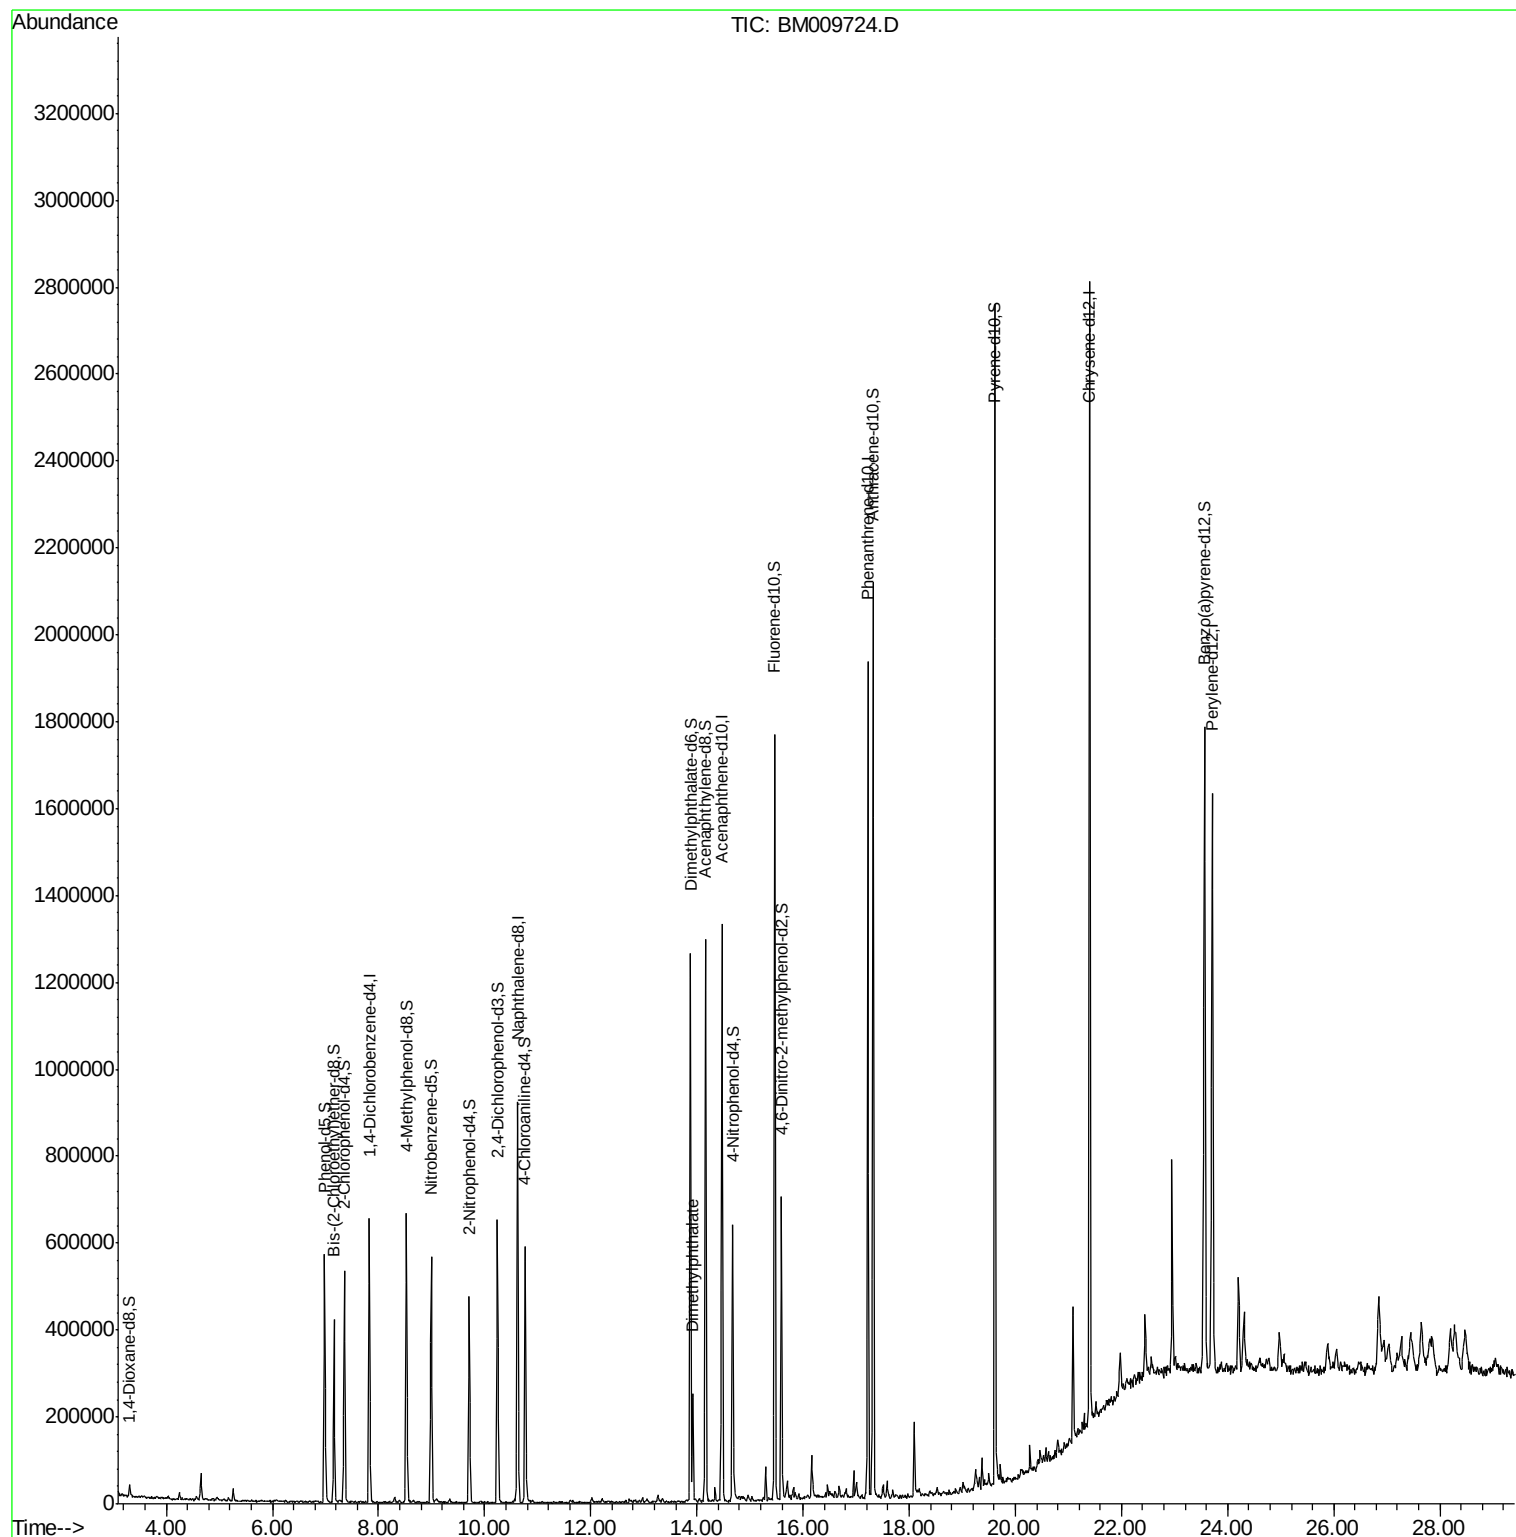

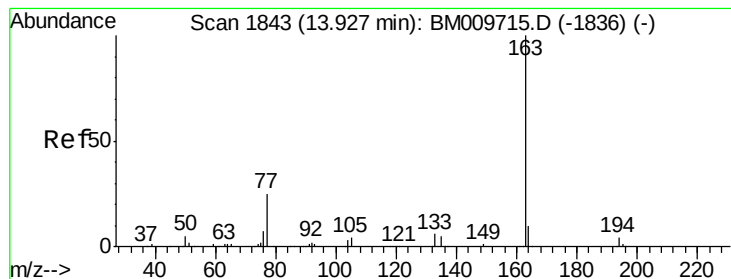

#44

Dimethylphthalate

Concen: 3.66 ng/ul

RT: 13.93 min Scan# 1843

Delta R.T. -0.00 min

Lab File: BM009724.D


Acq: 26 Apr 2017 17:36

Instrument :

BNA_M

ClientSampleId :

EME-TS001-01

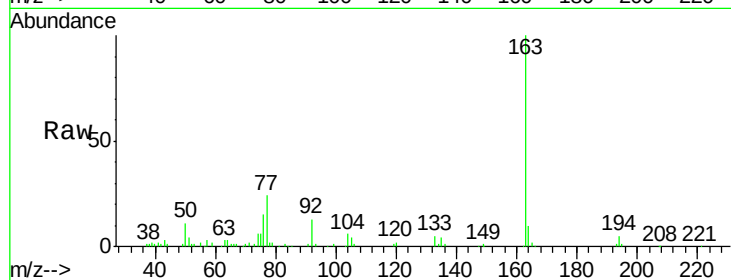

Tgt Ion:	163	Resp:	125628
Ion	Ratio	Lower	Upper
163	100		
194	4.8	3.0	4.6#
164	9.7	8.6	12.8

