

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042617\
 Data File : BM009725.D
 Acq On : 26 Apr 2017 18:12
 Operator : SJ/MA
 Sample : I2836-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EME-TS002-01

Quant Time: Apr 26 18:57:55 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 25 13:32:43 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	164134	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	702716	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	452422	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1098852	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1332760	20.00	ng/ul	0.00
83) Perylene-d12	23.72	264	1011723	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	13643	3.83	ng/uL	0.00
5) Phenol-d5	6.99	99	290761	16.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	217944	17.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	202556	17.86	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	237817	17.11	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	106412	18.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	113332	18.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	217070	18.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	275075	18.97	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	790523	20.09	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	945985	19.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	117181	15.43	ng/ul	0.00
57) Fluorene-d10	15.46	176	715339	20.14	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	114056	14.71	ng/ul	0.00
70) Anthracene-d10	17.32	188	1141757	20.24	ng/ul	0.00
76) Pyrene-d10	19.62	212	1370336	23.30	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1030380	20.94	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.93	163	147374	3.79	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042617\
Data File : BM009725.D
Acq On : 26 Apr 2017 18:12
Operator : SJ/MA
Sample : I2836-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EME-TS002-01

Quant Time: Apr 26 18:57:55 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 25 13:32:43 2017
Response via : Initial Calibration

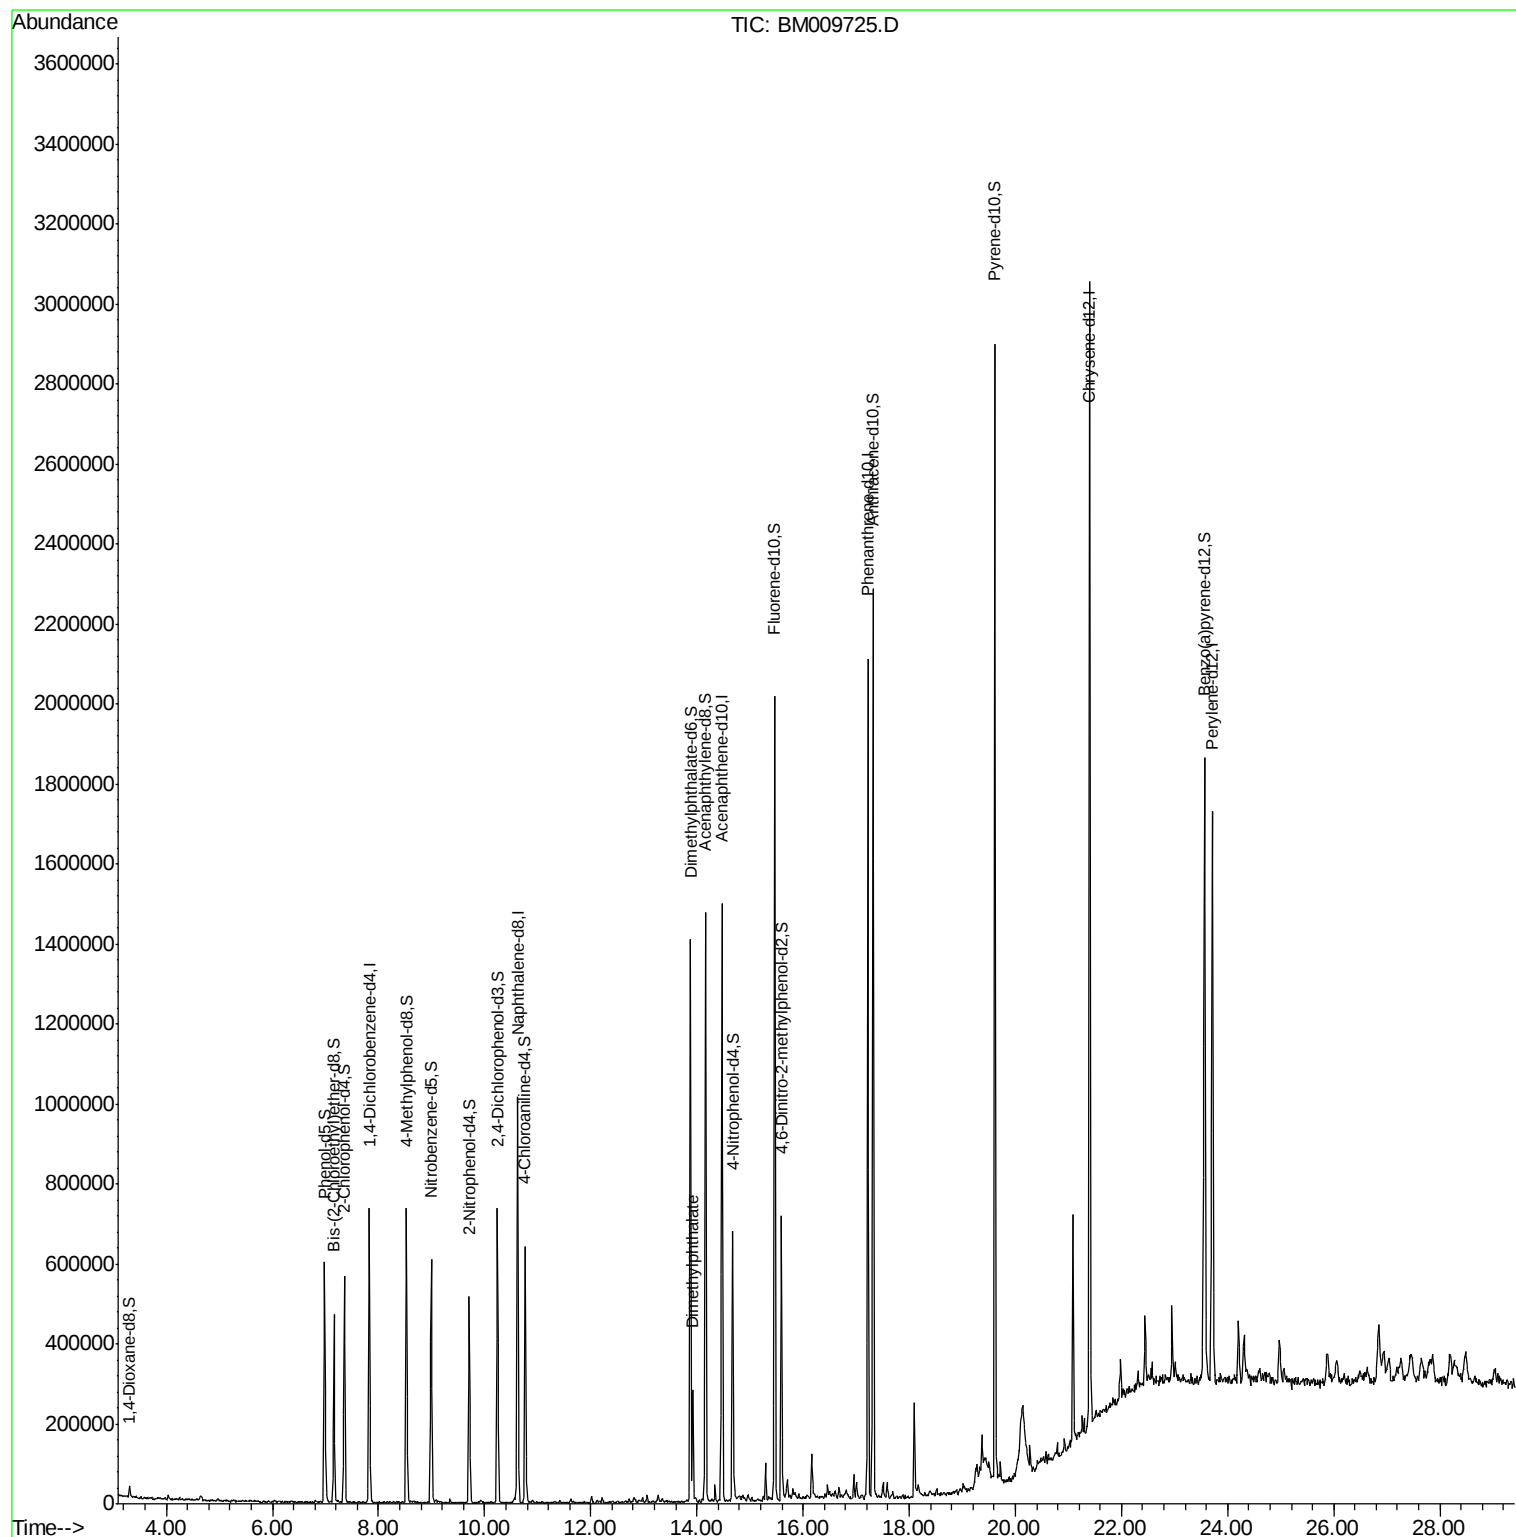

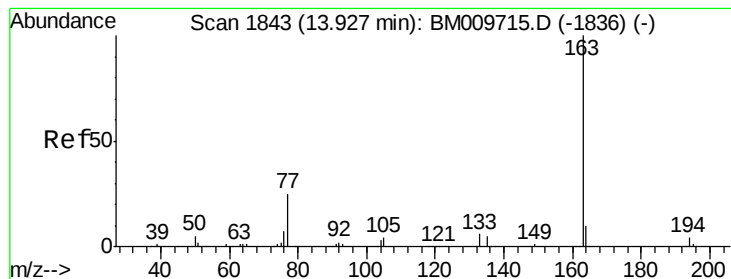

#44
 Dimethylphthalate
 Concen: 3.79 ng/ul
 RT: 13.93 min Scan# 1843
 Delta R.T. 0.00 min
 Lab File: BM009725.D
 Acq: 26 Apr 2017 18:12

Instrument :
 BNA_M
 ClientSampleId :
 EME-TS002-01

Tgt Ion:	163	Resp:	147374
Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.0	4.6
164	10.5	8.6	12.8

