


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042617\
Data File : BM009714.D
Acq On : 26 Apr 2017 11:34
Operator : SJ/MA
Sample : DFTPP06
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP06

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
Title : SVOA CALIBRATION
Last Update : Wed Nov 30 00:32:18 2016

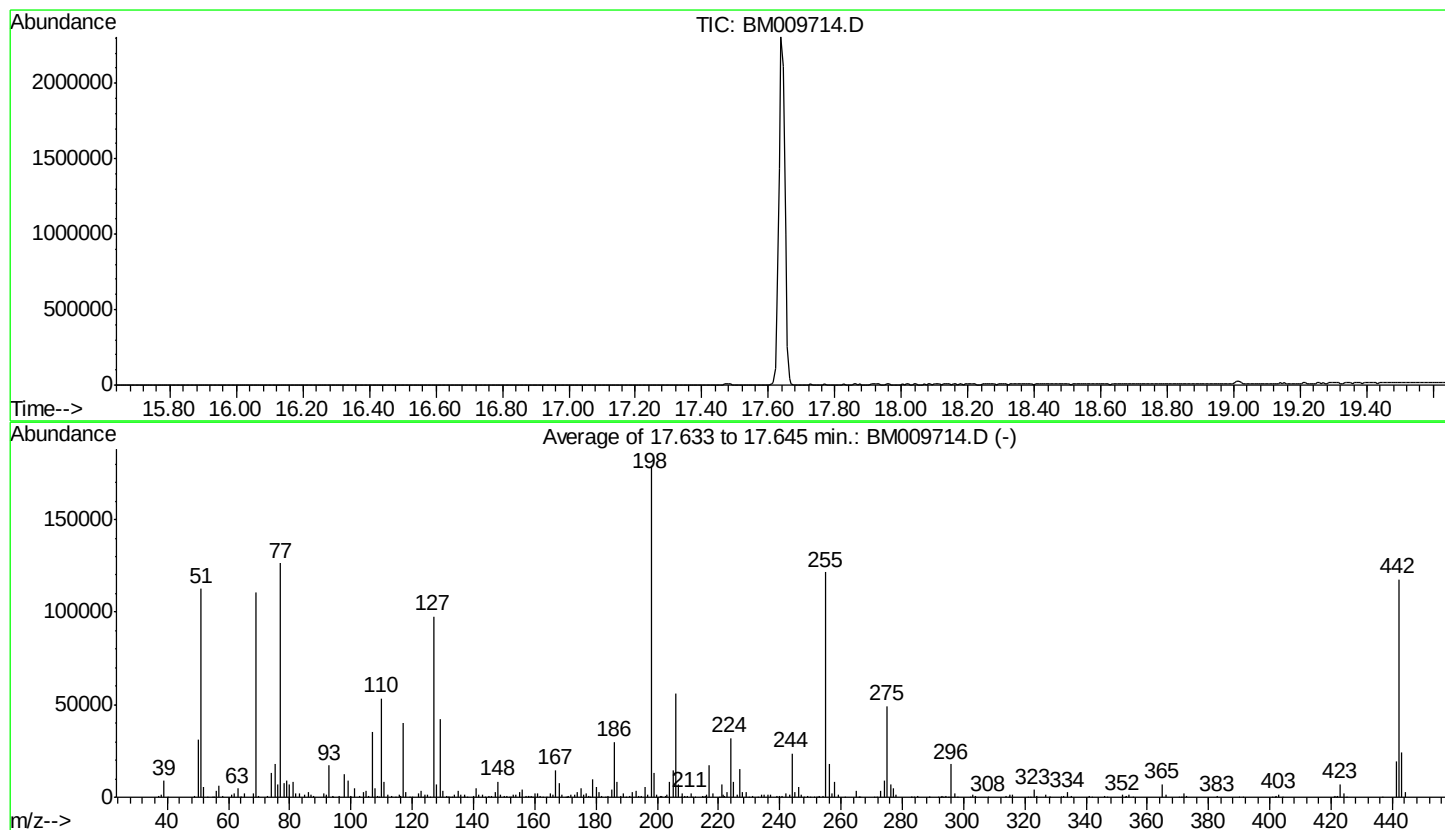

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	62.9	112672	PASS
68	69	0.00	2	1.8	2006	PASS
69	198	0.00	100	61.7	110474	PASS
70	69	0.00	2	0.6	707	PASS
127	198	10	80	54.6	97802	PASS
197	198	0.00	2	0.8	1478	PASS
198	198	100	100	100.0	179088	PASS
199	198	5	9	7.4	13316	PASS
275	198	10	60	27.4	49157	PASS
365	198	1	100	4.0	7237	PASS
441	443	0.01	100	80.4	19617	PASS
442	198	50	100	65.7	117720	PASS
443	442	15	24	20.7	24402	PASS

m/z	Abundance
37.10	431.0
38.10	1234.0
39.10	7828.0
40.00	782.0
44.00	486.0
49.10	473.0
50.00	25056.0
51.00	92824.0
52.00	5137.0
56.00	2345.0
57.00	5392.0
58.00	361.0
61.10	1231.0
62.00	1130.0
63.10	4141.0
63.90	570.0
65.10	1407.0
67.90	2277.0
69.00	93448.0
70.00	582.0
73.00	999.0
74.00	10974.0
75.00	14622.0
76.00	5279.0
77.10	106656.0
78.10	6309.0
79.00	7795.0
80.00	6026.0
81.00	6286.0
82.00	1584.0
83.00	1396.0
84.90	1066.0
86.00	2950.0
86.90	689.0
87.90	406.0
91.00	1496.0
91.80	1678.0
93.00	12753.0
93.90	924.0
96.10	783.0
98.00	9412.0
99.00	7000.0
99.80	397.0
101.00	4019.0
103.00	682.0
104.00	2534.0
105.00	2965.0
107.00	28816.0
108.00	4000.0
109.10	655.0
110.00	41264.0
111.00	7626.0
112.00	844.0
113.20	436.0
114.70	305.0
115.90	1728.0
117.00	30824.0
118.00	2257.0
122.00	1779.0
123.00	2375.0
123.80	1018.0
125.00	509.0
127.00	74728.0
128.00	5436.0
129.00	34368.0
130.00	2985.0
131.20	446.0
133.90	1651.0
134.90	3070.0
135.90	1139.0
136.90	1426.0
138.00	482.0
139.80	391.0
141.00	3632.0
141.80	1151.0
143.00	851.0
145.20	318.0
145.90	425.0
147.00	1987.0
148.00	7046.0
148.90	1229.0
151.20	329.0
151.80	863.0
153.00	1284.0
153.90	1070.0
155.00	2427.0
156.00	3475.0
157.20	505.0
158.00	786.0
159.10	662.0
160.00	1456.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

161.00	1639.0
162.00	961.0
163.70	343.0
164.80	1854.0
166.00	1255.0
167.00	10494.0
168.00	5637.0
169.00	1197.0
171.00	314.0
172.00	1014.0
172.90	1494.0
174.10	2234.0
175.10	3511.0
176.00	1447.0
177.00	1863.0
177.80	714.0
178.90	7178.0
180.00	4300.0
181.00	2328.0
181.80	511.0
183.90	632.0
184.90	2828.0
186.00	22896.0
187.00	6032.0
188.10	663.0
188.90	1416.0
191.00	819.0
191.90	2738.0
193.00	2524.0
194.00	607.0
195.00	352.0
195.90	4453.0
197.00	1683.0
197.90	129904.0
198.90	11253.0
199.90	656.0
201.10	616.0
201.50	718.0
202.80	1039.0
203.10	982.0
204.00	5413.0
205.00	9405.0
206.00	41872.0
207.00	6073.0
207.70	978.0
208.10	1157.0
208.90	872.0
210.10	576.0
210.90	1842.0
211.60	405.0
212.30	324.0
214.80	530.0
215.80	1323.0
216.90	11225.0
217.90	820.0
220.20	504.0
220.90	4391.0
221.70	1199.0
223.00	2141.0
224.00	21480.0
225.00	6541.0
225.90	1127.0
226.90	10439.0
228.00	1489.0
229.00	2210.0
231.10	620.0
233.90	1002.0
235.00	989.0
236.00	774.0
237.00	687.0
239.00	384.0
240.00	489.0
240.90	573.0
242.10	1075.0
243.10	1210.0
244.10	14735.0
245.00	2010.0
246.00	3508.0
247.00	836.0
252.80	733.0
254.10	508.0
255.00	83104.0
256.00	11484.0
257.00	1190.0
258.00	5659.0
258.90	1176.0
264.90	1948.0
265.70	475.0
266.20	349.0
273.00	2282.0
274.00	5217.0
275.00	30416.0
276.10	4444.0
277.00	3411.0
277.90	997.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

280.90	429.0
284.80	419.0
288.80	330.0
291.80	343.0
292.90	1049.0
294.10	384.0
296.00	11323.0
297.10	963.0
303.00	1195.0
303.70	331.0
314.00	649.0
314.80	935.0
316.00	434.0
321.00	312.0
322.90	2493.0
324.10	932.0
327.00	736.0
331.80	320.0
334.10	1062.0
335.10	640.0
341.10	311.0
345.90	350.0
352.00	616.0
352.90	826.0
354.10	1113.0
355.00	336.0
364.90	3491.0
366.00	816.0
372.00	1657.0
391.10	352.0
403.10	825.0
404.10	529.0
420.80	324.0
422.10	719.0
423.00	3724.0
424.10	1675.0
441.10	9595.0
442.00	63496.0
443.10	13327.0
444.10	628.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

m/z	Abundance
37.00	626.0
38.00	1833.0
39.10	10635.0
40.00	1125.0
48.90	587.0
49.20	519.0
50.00	36768.0
51.00	138176.0
52.00	5984.0
52.90	359.0
54.90	367.0
56.00	3711.0
57.00	6826.0
57.90	314.0
60.90	1990.0
62.00	3114.0
63.00	5418.0
64.10	596.0
65.00	2811.0
68.00	1836.0
69.00	132544.0
69.90	951.0
73.00	1413.0
74.00	14389.0
75.10	21408.0
76.00	8841.0
77.10	147776.0
78.10	9571.0
79.00	9756.0
80.00	6956.0
80.90	11252.0
82.00	2963.0
83.10	1646.0
84.90	1004.0
86.00	2959.0
87.00	1864.0
87.80	602.0
90.90	2077.0
92.00	2564.0
93.00	19808.0
94.10	859.0
96.00	1206.0
98.00	15887.0
99.00	11364.0
100.10	1263.0
101.00	5247.0
102.80	1550.0
104.00	2893.0
105.00	4195.0
105.90	1101.0
107.00	41896.0
108.00	5994.0
108.80	1018.0
110.00	62640.0
110.90	9262.0
111.90	959.0
116.10	2237.0
117.00	48696.0
117.90	2949.0
118.90	420.0
119.80	402.0
122.00	3188.0
122.90	4019.0
124.00	3022.0
125.00	2046.0
127.00	116040.0
128.00	8846.0
129.00	50488.0
130.00	3766.0
131.00	706.0
131.80	621.0
133.90	1327.0
135.00	3707.0
135.80	2011.0
137.10	2095.0
138.00	495.0
139.90	518.0
141.10	6587.0
141.80	1255.0
143.00	1659.0
145.10	411.0
146.00	1009.0
147.10	2832.0
148.00	8981.0
148.90	1950.0
150.00	669.0
151.00	608.0
153.00	2140.0
154.00	2205.0
155.00	3359.0
156.10	4520.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

157.00	1205.0
157.80	1591.0
158.70	859.0
160.00	2534.0
160.90	2154.0
161.90	1023.0
163.70	552.0
164.90	3103.0
165.90	1636.0
166.90	17200.0
168.00	9966.0
168.90	1466.0
170.80	985.0
172.00	1172.0
173.00	1951.0
174.00	3170.0
175.00	5831.0
176.00	2145.0
176.90	2411.0
178.00	1082.0
178.90	10332.0
180.00	7259.0
180.90	2952.0
181.90	674.0
183.90	696.0
184.90	5186.0
186.00	35472.0
187.00	9422.0
188.10	1360.0
188.90	2288.0
189.80	506.0
190.80	1134.0
191.90	3344.0
193.00	4534.0
193.90	830.0
195.00	398.0
196.00	5483.0
196.90	1710.0
197.90	215936.0
198.90	15356.0
200.00	1410.0
200.90	716.0
201.50	492.0
202.90	1866.0
204.00	8950.0
205.00	17496.0
206.00	67704.0
207.00	9536.0
208.00	3444.0
209.00	912.0
209.90	1212.0
211.00	3220.0
212.20	486.0
215.00	762.0
216.00	2363.0
216.90	19416.0
218.00	2750.0
221.00	8434.0
221.70	2195.0
223.00	2998.0
224.00	38944.0
225.00	9855.0
226.00	1483.0
227.00	17752.0
228.00	2685.0
229.00	3908.0
230.00	509.0
231.00	1152.0
232.90	380.0
233.90	1243.0
235.00	1574.0
236.10	1759.0
236.90	1487.0
239.00	504.0
240.00	1046.0
240.80	1170.0
242.00	2004.0
242.90	1617.0
244.00	28560.0
245.00	3709.0
246.00	5896.0
246.90	1297.0
248.90	1112.0
250.10	445.0
252.10	782.0
253.00	488.0
254.00	1143.0
255.00	140288.0
256.00	20880.0
257.00	2449.0
258.00	9830.0
258.90	1964.0
261.10	551.0
265.00	4539.0
265.90	457.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

270.80	364.0
271.90	485.0
273.00	4279.0
273.90	10417.0
275.00	59776.0
276.00	7392.0
277.00	6405.0
278.00	1617.0
283.10	629.0
283.90	406.0
284.90	640.0
289.00	331.0
293.00	1036.0
293.90	463.0
295.10	449.0
296.00	20616.0
297.00	2389.0
302.10	367.0
302.90	1549.0
304.00	793.0
308.10	308.0
314.10	843.0
315.00	2351.0
316.00	1176.0
321.80	455.0
323.00	4987.0
323.90	843.0
326.90	1348.0
327.90	520.0
332.00	424.0
332.90	369.0
334.00	3141.0
335.00	1071.0
341.00	455.0
342.00	596.0
346.00	798.0
352.00	1759.0
353.20	593.0
354.00	1517.0
355.00	392.0
365.00	9019.0
366.00	1477.0
371.00	416.0
371.90	2242.0
372.90	688.0
383.00	557.0
391.10	356.0
401.80	623.0
403.00	1417.0
404.10	391.0
421.00	1295.0
421.80	690.0
423.10	7907.0
424.10	2576.0
436.90	365.0
441.10	22232.0
442.10	132992.0
443.10	28952.0
444.10	3562.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

m/z	Abundance
37.00	398.0
38.10	1422.0
39.10	7554.0
40.10	742.0
43.90	665.0
48.90	613.0
50.00	31160.0
51.10	107016.0
52.10	5892.0
55.10	704.0
55.90	3933.0
57.10	6301.0
58.00	592.0
60.90	1660.0
61.90	1863.0
63.00	4190.0
63.90	396.0
65.00	2410.0
68.00	1905.0
69.00	105432.0
69.90	590.0
72.90	1159.0
74.10	13218.0
75.00	18944.0
76.00	6662.0
77.10	124344.0
78.10	7075.0
79.00	9982.0
80.00	8055.0
81.00	7277.0
82.10	1749.0
83.00	2253.0
84.90	1392.0
85.90	2017.0
87.00	1237.0
88.00	330.0
90.90	2243.0
91.90	2218.0
93.00	19080.0
93.90	659.0
96.10	573.0
98.00	11904.0
99.00	8005.0
100.10	514.0
101.10	5298.0
103.00	955.0
104.10	2150.0
105.00	2350.0
105.80	902.0
107.00	35216.0
108.00	5409.0
108.80	986.0
110.00	56776.0
111.00	7958.0
112.00	1464.0
113.00	690.0
115.90	2054.0
117.00	40976.0
118.00	3498.0
119.00	357.0
119.90	543.0
122.00	1813.0
123.00	3451.0
123.90	2007.0
125.10	1674.0
126.00	881.0
127.00	102640.0
128.00	6754.0
129.00	42544.0
130.00	3766.0
131.00	545.0
132.00	336.0
133.00	402.0
133.90	1341.0
135.00	4572.0
135.90	919.0
136.90	1927.0
140.00	664.0
141.00	4457.0
141.80	1565.0
142.90	1125.0
143.80	347.0
145.00	570.0
145.90	1267.0
147.00	2675.0
148.00	8962.0
149.00	1309.0
150.10	499.0
151.00	547.0
152.00	687.0
153.00	1820.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

154.00	1741.0
155.00	3425.0
156.00	5446.0
157.00	1114.0
158.10	1177.0
158.80	841.0
160.00	2305.0
161.00	2270.0
161.90	918.0
162.70	397.0
165.00	2291.0
166.10	1425.0
167.00	16154.0
168.10	7852.0
168.90	1270.0
170.00	374.0
170.60	382.0
171.00	451.0
171.90	1305.0
173.10	1016.0
174.00	2603.0
175.00	5817.0
175.80	760.0
176.80	1894.0
177.80	620.0
179.00	11051.0
180.00	6138.0
181.00	2817.0
181.90	558.0
183.20	530.0
184.00	1821.0
185.00	4314.0
186.00	30944.0
187.00	9334.0
188.10	698.0
188.90	2358.0
189.80	450.0
190.80	947.0
192.00	2558.0
193.10	3042.0
193.90	889.0
194.90	423.0
195.90	5855.0
197.00	1043.0
198.00	191424.0
198.90	13339.0
199.90	1300.0
201.60	1586.0
203.00	2371.0
204.00	9761.0
205.00	16800.0
206.00	59456.0
207.00	9059.0
207.90	1809.0
208.90	1330.0
209.90	1332.0
211.00	2093.0
211.70	475.0
214.90	924.0
216.00	1829.0
216.90	20264.0
218.00	2749.0
221.00	7104.0
222.00	1813.0
222.90	3331.0
224.00	35720.0
224.90	7613.0
225.90	1274.0
227.00	17656.0
227.90	3204.0
228.80	2861.0
229.90	484.0
230.90	1138.0
233.90	1178.0
234.90	1608.0
236.10	1523.0
236.90	1855.0
239.10	640.0
239.80	496.0
240.80	1104.0
242.00	2317.0
243.10	1566.0
244.00	27512.0
245.00	3304.0
246.00	6830.0
246.90	1264.0
248.00	304.0
249.00	1345.0
251.10	405.0
252.00	308.0
252.90	1110.0
254.00	1208.0
255.00	141504.0
256.00	21472.0
257.00	1654.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

258.00	10141.0
258.90	1741.0
260.90	388.0
264.90	3737.0
266.10	735.0
271.80	330.0
272.90	3781.0
274.00	11300.0
275.00	57280.0
276.00	8756.0
277.00	5143.0
278.00	1225.0
282.80	865.0
283.90	489.0
285.00	1127.0
288.90	324.0
292.70	539.0
293.20	844.0
294.00	554.0
295.00	496.0
296.00	21120.0
297.00	3124.0
297.90	330.0
303.00	2397.0
304.00	1139.0
314.00	910.0
315.00	2303.0
316.00	1743.0
320.90	470.0
323.00	4963.0
324.00	1086.0
327.00	1502.0
328.10	1089.0
332.00	561.0
332.80	743.0
334.00	3751.0
334.90	711.0
340.90	370.0
345.90	1425.0
347.00	443.0
352.10	1630.0
353.10	912.0
354.00	1409.0
355.10	306.0
365.00	9203.0
365.90	1843.0
370.10	330.0
370.90	338.0
372.00	2065.0
372.90	670.0
383.00	774.0
390.10	388.0
400.80	301.0
402.00	1454.0
403.00	1943.0
421.10	1522.0
422.00	886.0
423.00	9828.0
424.10	2239.0
425.00	314.0
441.10	27024.0
442.00	156672.0
443.10	30928.0
444.00	3240.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06

Scan 2468 (17.604 min): BM009714.D
DFTPP06

m/z	Abundance
40.00	657.0
44.10	815.0
73.10	517.0
190.80	364.0
207.00	967.0
280.90	331.0

Instrument :
BNA_M
ClientSampleId :
DFTPP06