

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042618\
 Data File : BM014854.D
 Acq On : 26 Apr 2018 10:48
 Operator : SJ/JU
 Sample : PB108614BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Apr 27 01:07:13 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 27 01:05:24 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.50	152	257350	20.00	ng/ul	0.00
18) Naphthalene-d8	11.35	136	1087976	20.00	ng/ul	0.00
35) Acenaphthene-d10	15.10	164	569209	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.82	188	1268614	20.00	ng/ul	0.00
75) Chrysene-d12	21.90	240	1338829	20.00	ng/ul	0.00
83) Perylene-d12	24.39	264	1404695	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.64	96	37716	6.40	ng/uL	0.00
5) Phenol-d5	7.62	99	603750	30.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.80	67	411667	32.27	ng/ul	0.00
9) 2-Chlorophenol-d4	8.02	132	496336	29.82	ng/ul	0.00
13) 4-Methylphenol-d8	9.20	113	482724	30.43	ng/ul	0.00
19) Nitrobenzene-d5	9.68	128	232057	29.50	ng/ul	0.00
22) 2-Nitrophenol-d4	10.41	143	236814	30.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.95	165	444089	27.90	ng/ul	0.00
29) 4-Chloroaniline-d4	11.47	131	692451	44.08	ng/ul	0.00
43) Dimethylphthalate-d6	14.50	166	1520843	34.23	ng/ul	0.00
46) Acenaphthylene-d8	14.80	160	1686770	30.74	ng/ul	0.00
51) 4-Nitrophenol-d4	15.26	143	265168	32.16	ng/ul	0.00
57) Fluorene-d10	16.08	176	1271894	32.91	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.18	200	156858	22.85	ng/ul	0.00
70) Anthracene-d10	17.92	188	2003636	33.89	ng/ul	0.00
76) Pyrene-d10	20.16	212	2195767	34.67	ng/ul	0.00
87) Benzo(a)pyrene-d12	24.23	264	2515031	36.44	ng/ul	0.00
Target Compounds						
15) N-Nitroso-di-n-propylamine	9.19	70	12330	1.022	ng/ul#	1
45) 2,6-Dinitrotoluene	14.50	165	9705	1.232	ng/ul#	27


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042618\
Data File : BM014854.D
Acq On : 26 Apr 2018 10:48
Operator : SJ/JU
Sample : PB108614BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Apr 27 01:07:13 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM041918.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 27 01:05:24 2018
Response via : Initial Calibration

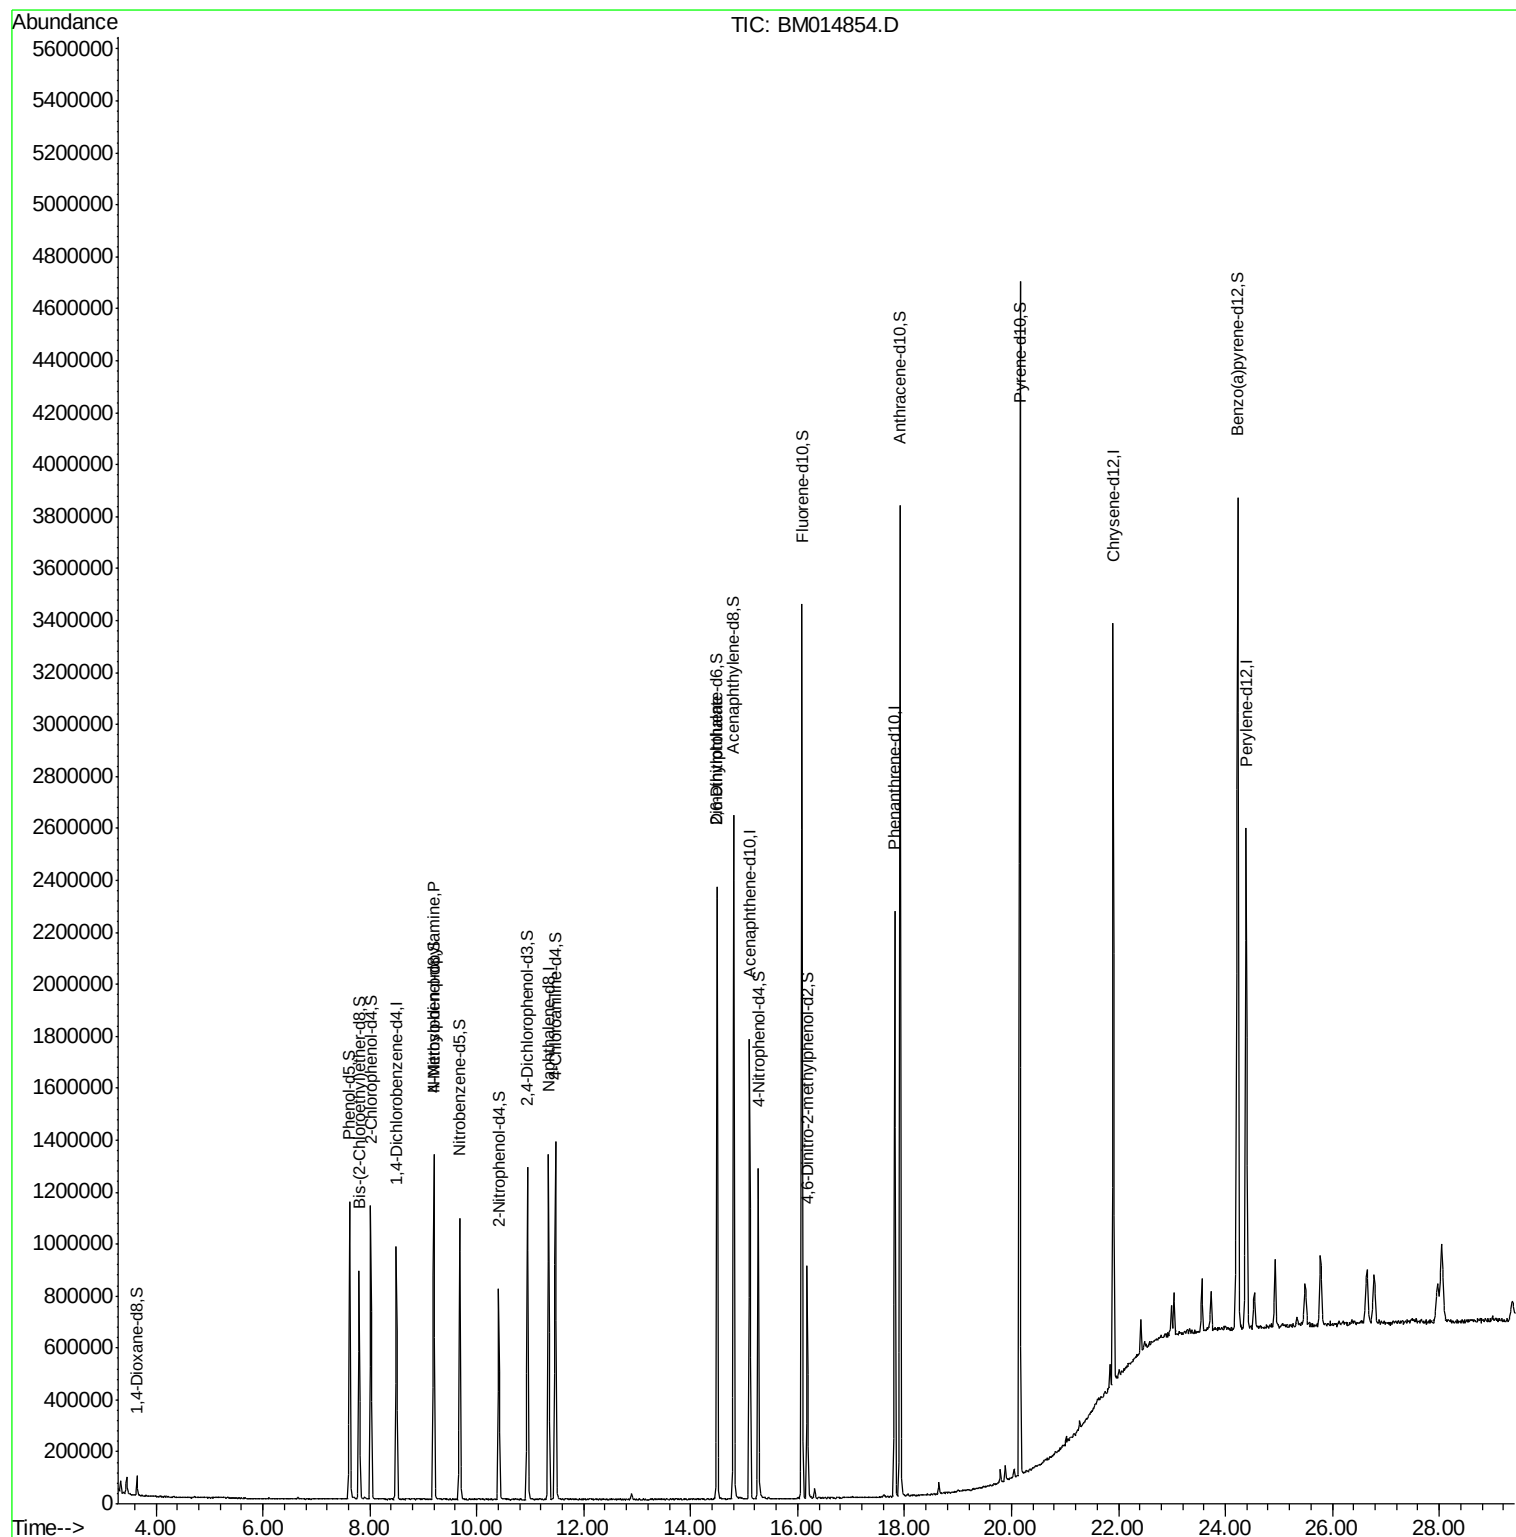

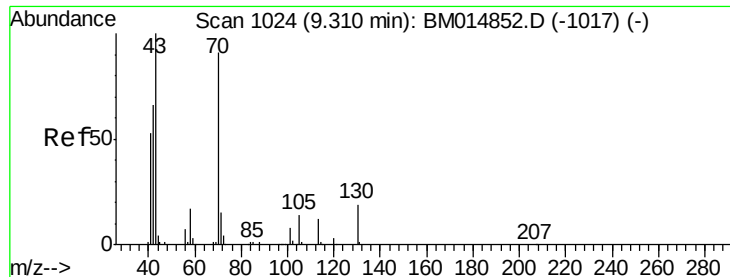

#15

N-Nitroso-di-n-propylamine

Concen: 1.022 ng/ul

RT: 9.19 min Scan# 1004

Delta R.T. -0.12 min


Lab File: BM014854.D

Acq: 26 Apr 2018 10:48




Instrument :

BNA_M

ClientSampled :

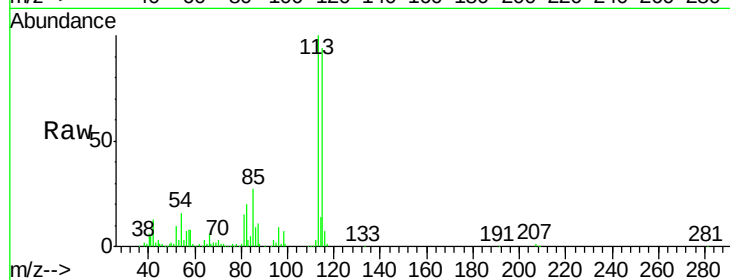

Tot Ion:	70	Resp:	12330
Ion	Ratio	Lower	Upper
70	100		
42	467.7	76.0	114.0#
101	0.0	6.7	10.1#
130	0.0	14.6	22.0#

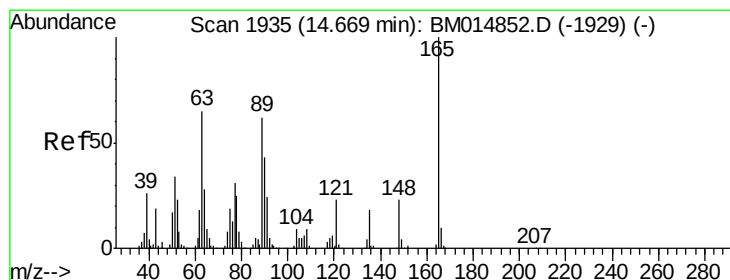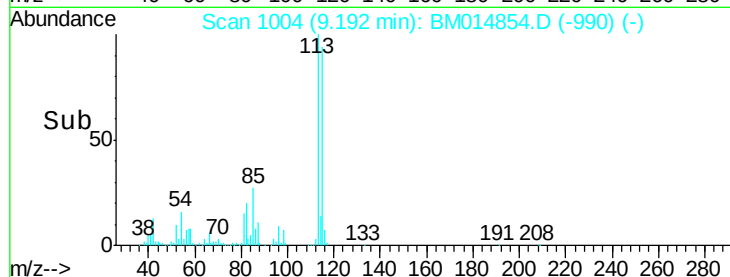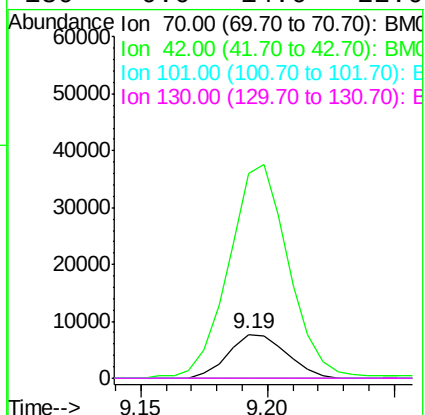

#45

2,6-Dinitrotoluene

Concen: 1.232 ng/ul

RT: 14.50 min Scan# 1906

Delta R.T. -0.17 min

Lab File: BM014854.D

Acq: 26 Apr 2018 10:48

Tgt Ion:	165	Resp:	9705
Ion	Ratio	Lower	Upper
165	100		
89	0.0	52.6	79.0#
121	34.8	14.6	22.0#

