
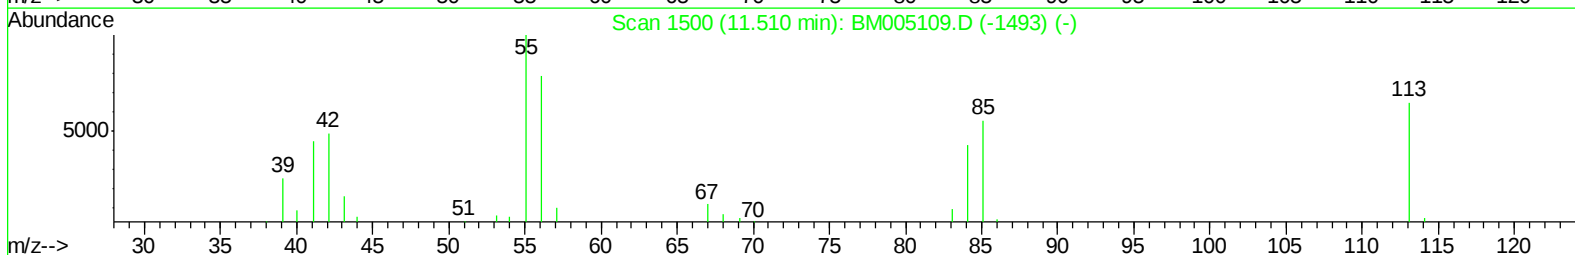
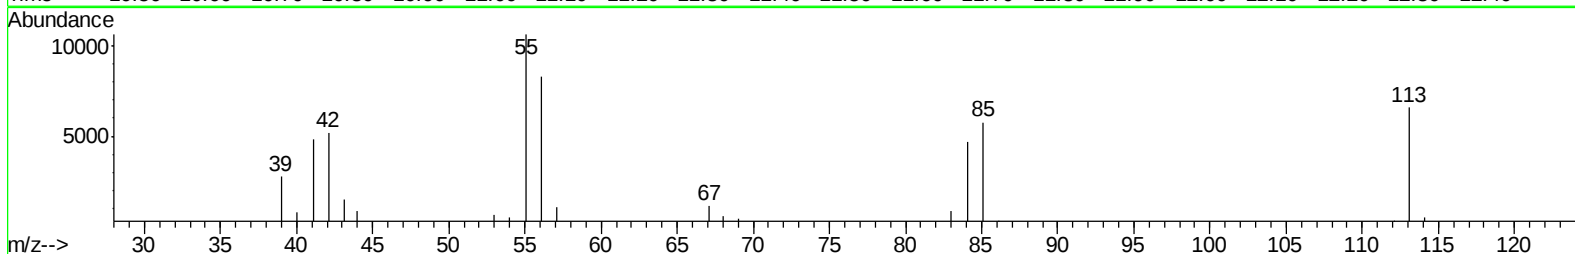


Data Path : Z:\HPCHEM1\BNA_M\Data\BM042816\
Data File : BM005117.D
Acq On : 28 Apr 2016 17:14
Operator : UM/SJ
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Apr 29 02:22:38 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 29 02:20:37 2016
Response via : Initial Calibration

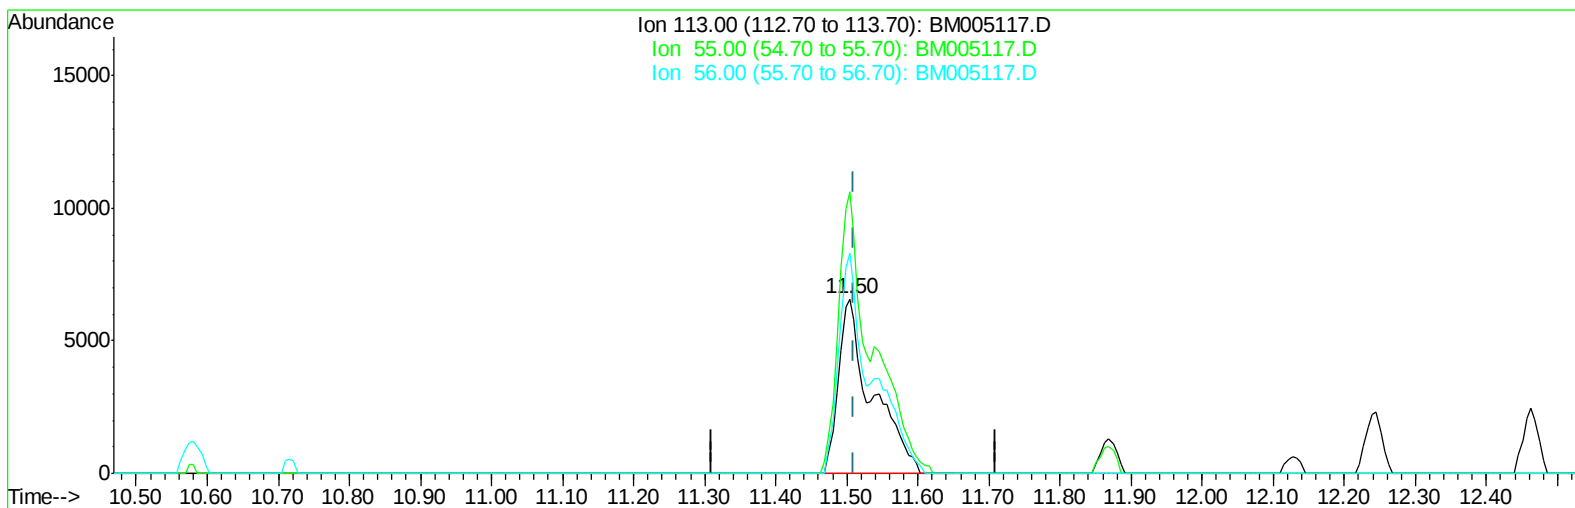

TIC: BM005117.D

(32) Caprolactam

11.504min (-0.006) 21.03ng/ul m

response 21449

Ion	Exp%	Act%
113.00	100	100
55.00	146.20	161.22
56.00	109.60	125.76
0.00	0.00	0.00