

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042716\
 Data File : BM005100.D
 Acq On : 27 Apr 2016 17:02
 Operator : UM/SJ
 Sample : H2584-19
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7K5

Manual Integrations
 APPROVED

sohil
 4/28/2016 1:41:30 PM

Quant Time: Apr 28 04:35:05 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 28 04:13:24 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.80	152	68039	20.00	ng/ul	0.00
18) Naphthalene-d8	10.59	136	317711	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.44	164	201207	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.19	188	465253	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	497950	20.00	ng/ul	0.00
83) Perylene-d12	23.66	264	390431	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	5572	4.16	ng/uL	0.00
5) Phenol-d5	6.97	99	125810	22.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.13	67	69510	21.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.33	132	95988	21.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.50	113	105951	22.20	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	45315	20.59	ng/ul	0.00
22) 2-Nitrophenol-d4	9.67	143	53936	21.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.21	165	102113	21.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	145731	26.66	ng/ul	0.00
43) Dimethylphthalate-d6	13.85	166	352976	22.21	ng/ul	0.00
46) Acenaphthylene-d8	14.13	160	421793	22.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.65	143	48167m	17.34	ng/ul	0.00
57) Fluorene-d10	15.43	176	314172	22.50	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.55	200	31601	11.94	ng/ul	0.00
70) Anthracene-d10	17.28	188	493233	23.64	ng/ul	0.00
76) Pyrene-d10	19.58	212	564960	24.92	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	427653	24.45	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.89	163	69453	4.36	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM042716\
Data File : BM005100.D
Acq On : 27 Apr 2016 17:02
Operator : UM/SJ
Sample : H2584-19
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BC7K5

Manual Integrations
APPROVED

sohil
4/28/2016 1:41:30 PM

Quant Time: Apr 28 04:35:05 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 28 04:13:24 2016
Response via : Initial Calibration

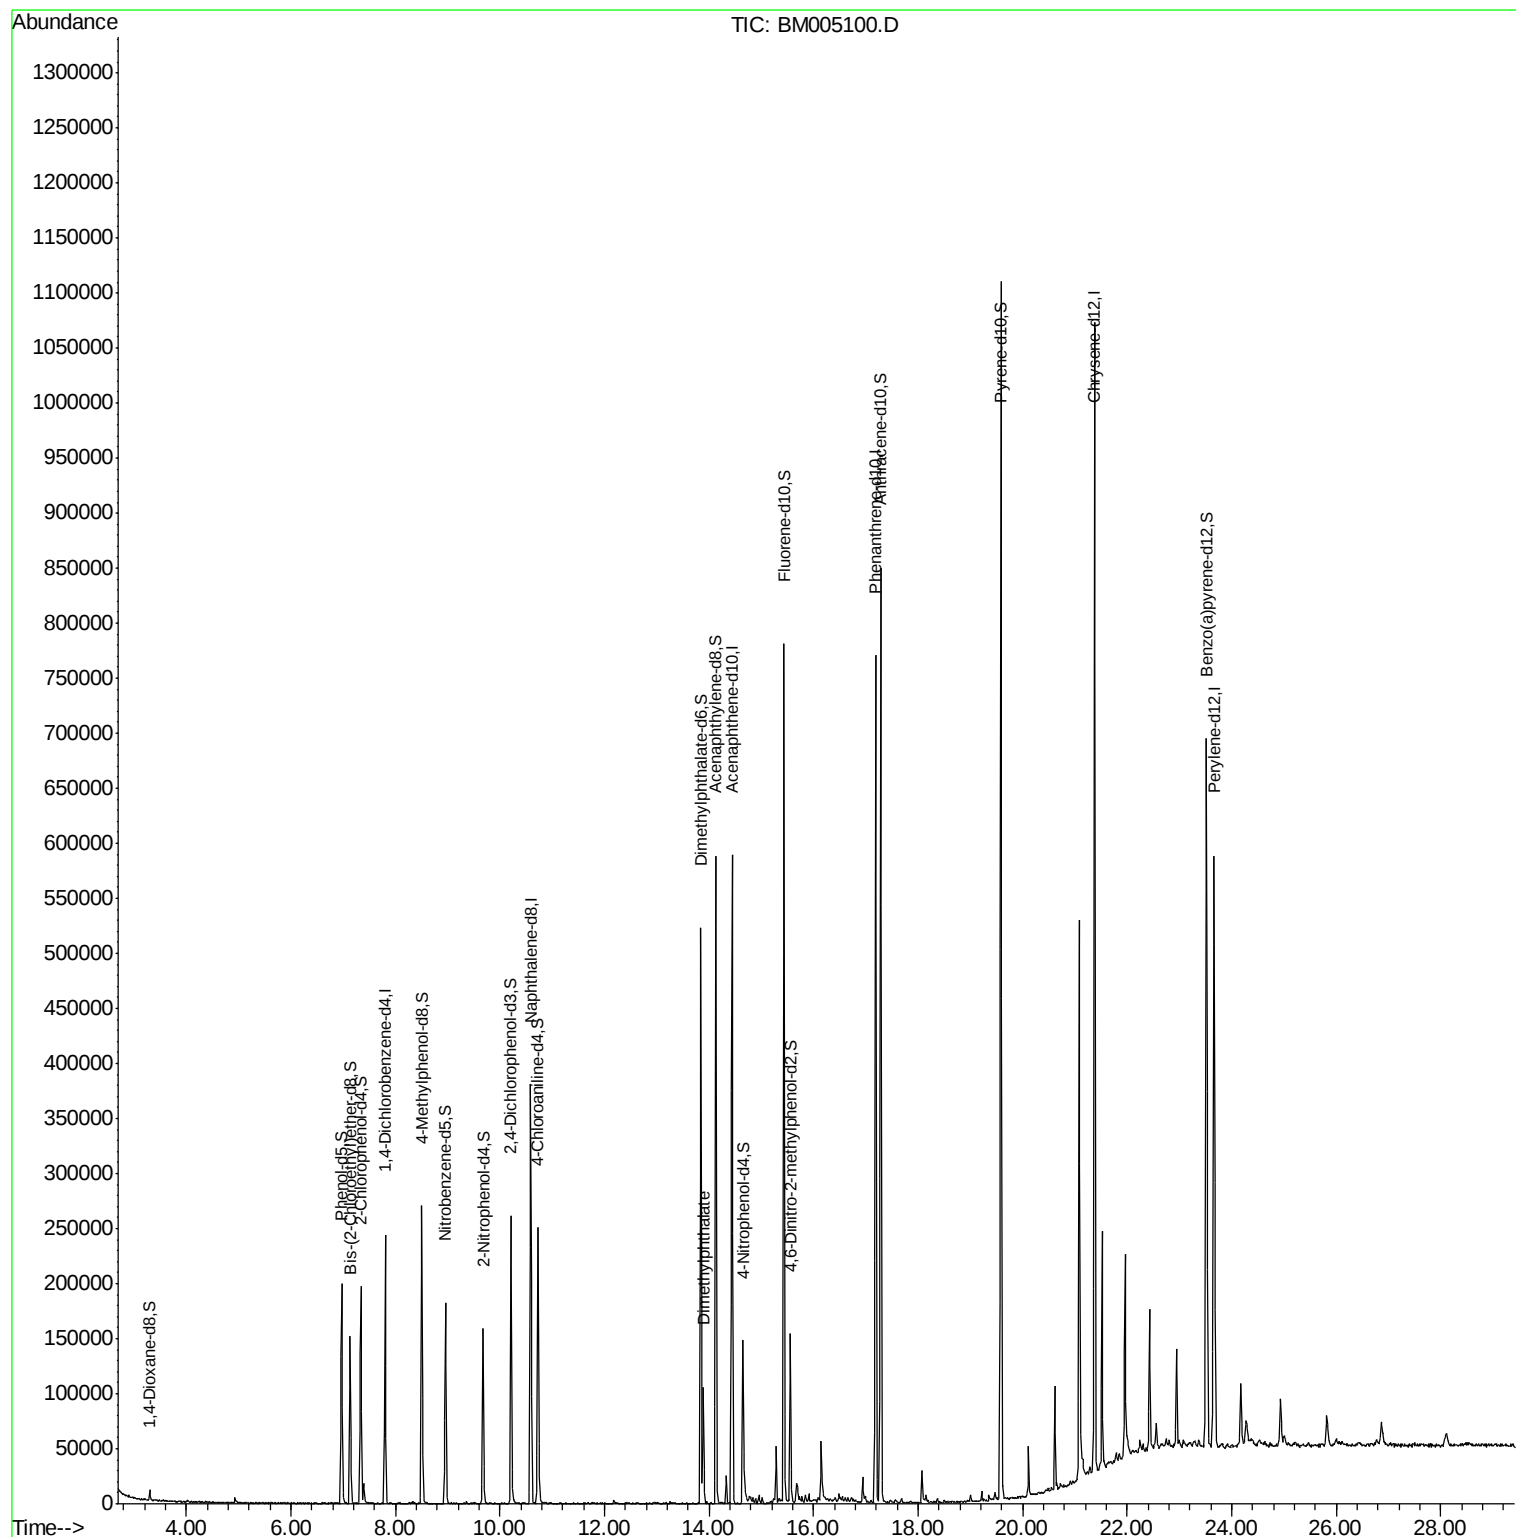

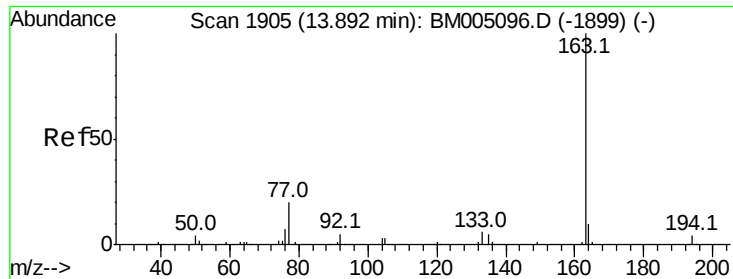

#44

Dimethylphthalate

Concen: 4.36 ng/ul

RT: 13.89 min Scan# 1905

Delta R.T. 0.00 min

Lab File: BM005100.D


Acq: 27 Apr 2016 17:02

Instrument :

BNA_M

ClientSampleId :

BC7K5

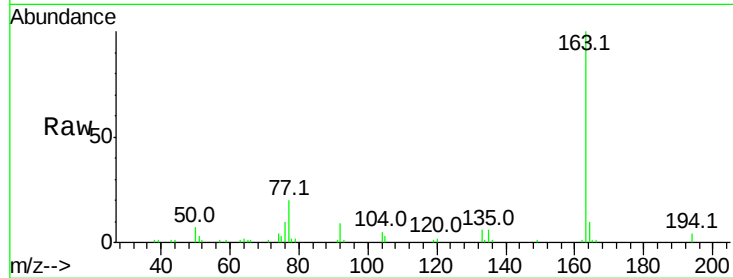

Tot Ion:	163	Resp:	69453
Ion Ratio	Lower	Upper	
163	100		
194	4.0	3.3	4.9
164	9.7	8.2	12.2

Manual Integrations
APPROVED

sohil
4/28/2016 1:41:30 PM

