

Data Path : Z:\HPCHEM1\BNA_M\Data\BM042717\
 Data File : BM009733.D
 Acq On : 27 Apr 2017 10:15
 Operator : SJ/MA
 Sample : PB98492BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK92

Quant Time: Apr 27 18:12:21 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 27 18:07:34 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	118362	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	505065	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	326415	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	789711	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	924794	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	699831	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	20906	8.13	ng/uL	0.00
5) Phenol-d5	6.99	99	417922	32.50	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	307845	35.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	296869	36.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	329407	32.86	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	150858	36.70	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	166459	38.49	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	293343	33.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	427447	41.01	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	1051616	37.04	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1277069	37.29	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	177087	32.32	ng/ul	0.00
57) Fluorene-d10	15.46	176	958700	37.40	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	172252	30.92	ng/ul	0.00
70) Anthracene-d10	17.32	188	1529820	37.73	ng/ul	0.00
76) Pyrene-d10	19.62	212	1729093	42.37	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1279613	37.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.53	70	10684	1.04	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\Data\BM042717\
Data File : BM009733.D
Acq On : 27 Apr 2017 10:15
Operator : SJ/MA
Sample : PB98492BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK92

Quant Time: Apr 27 18:12:21 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 27 18:07:34 2017
Response via : Initial Calibration

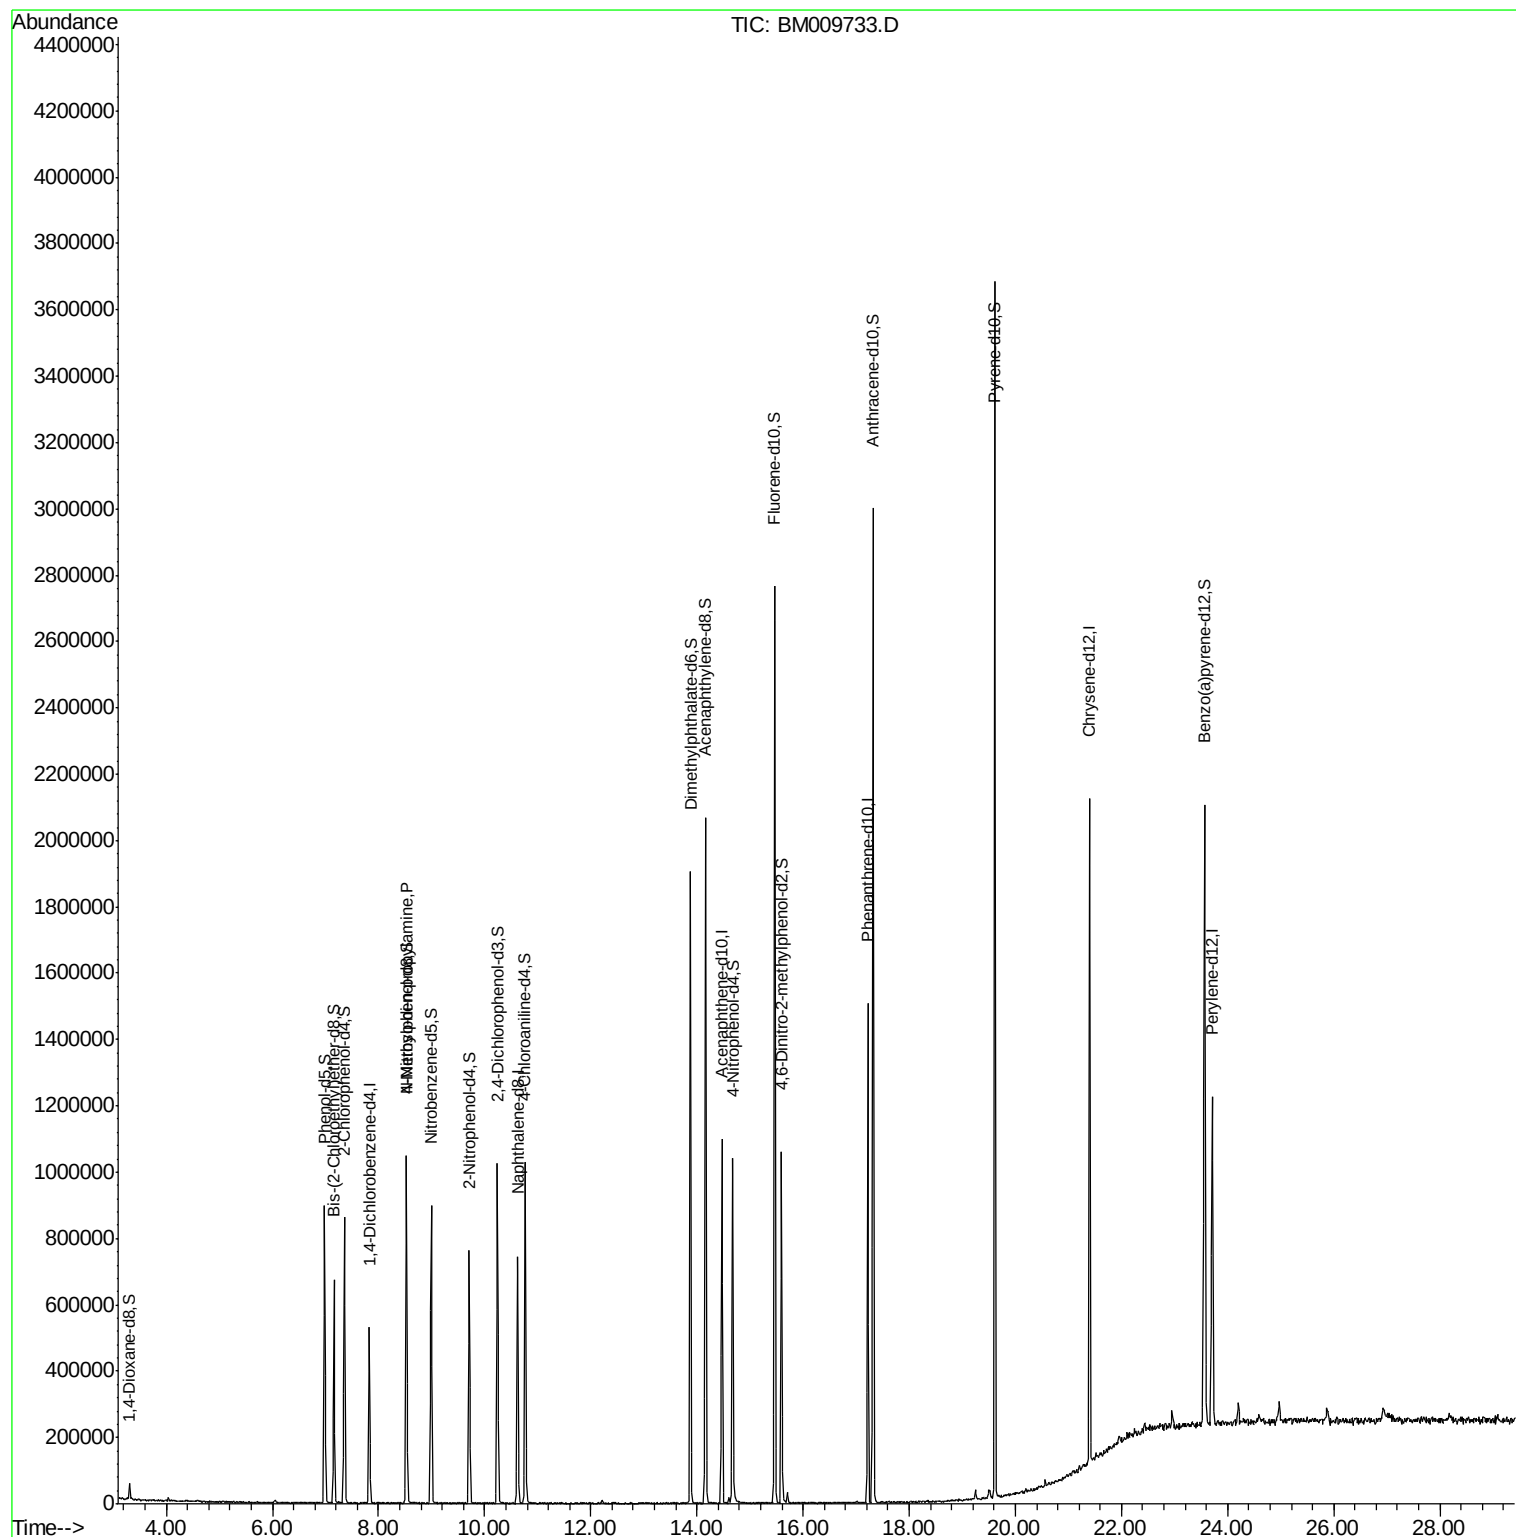

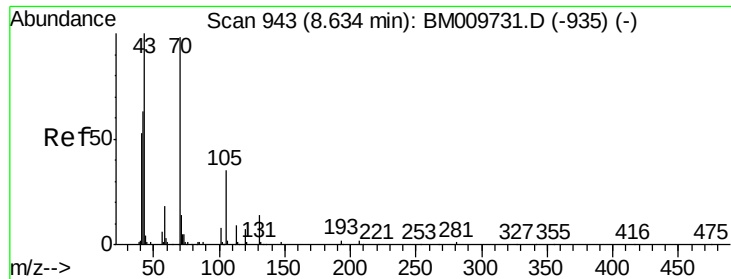

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.04 ng/ul
 RT: 8.53 min Scan# 925
 Delta R.T. -0.11 min
 Lab File: BM009733.D
 Acq: 27 Apr 2017 10:15

Instrument :
 BNA_M
 ClientSampleId :
 SBLK92

Tgt Ion: 70 Resp: 10684
 Ion Ratio Lower Upper
 70 100
 42 373.1 64.2 96.2#
 101 0.0 5.1 7.7#
 130 0.0 8.3 12.5#

