

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009734.D
 Acq On : 27 Apr 2017 10:51
 Operator : SJ/MA
 Sample : I2809-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHTC1

Quant Time: Apr 27 18:13:54 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 27 18:07:34 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.83	152	119897	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	511517	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	332922	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	811790	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1110157	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	1055467	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	14334	5.51	ng/uL	0.00
5) Phenol-d5	6.99	99	77205	5.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	256833	28.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	196730	23.74	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	147420	14.52	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	132510	31.83	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	144368	32.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	243414	27.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	17199	1.63	ng/ul	0.01
43) Dimethylphthalate-d6	13.88	166	974794	33.66	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1164005	33.33	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	29057	5.20	ng/ul	0.00
57) Fluorene-d10	15.46	176	902425	34.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.60	200	165552	28.90	ng/ul	0.00
70) Anthracene-d10	17.32	188	1521253	36.50	ng/ul	0.00
76) Pyrene-d10	19.62	212	1835942	37.47	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1871537	36.46	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
56) Diethylphthalate	15.29	149	36280	1.16	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009734.D
Acq On : 27 Apr 2017 10:51
Operator : SJ/MA
Sample : I2809-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHTC1

Quant Time: Apr 27 18:13:54 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 27 18:07:34 2017
Response via : Initial Calibration

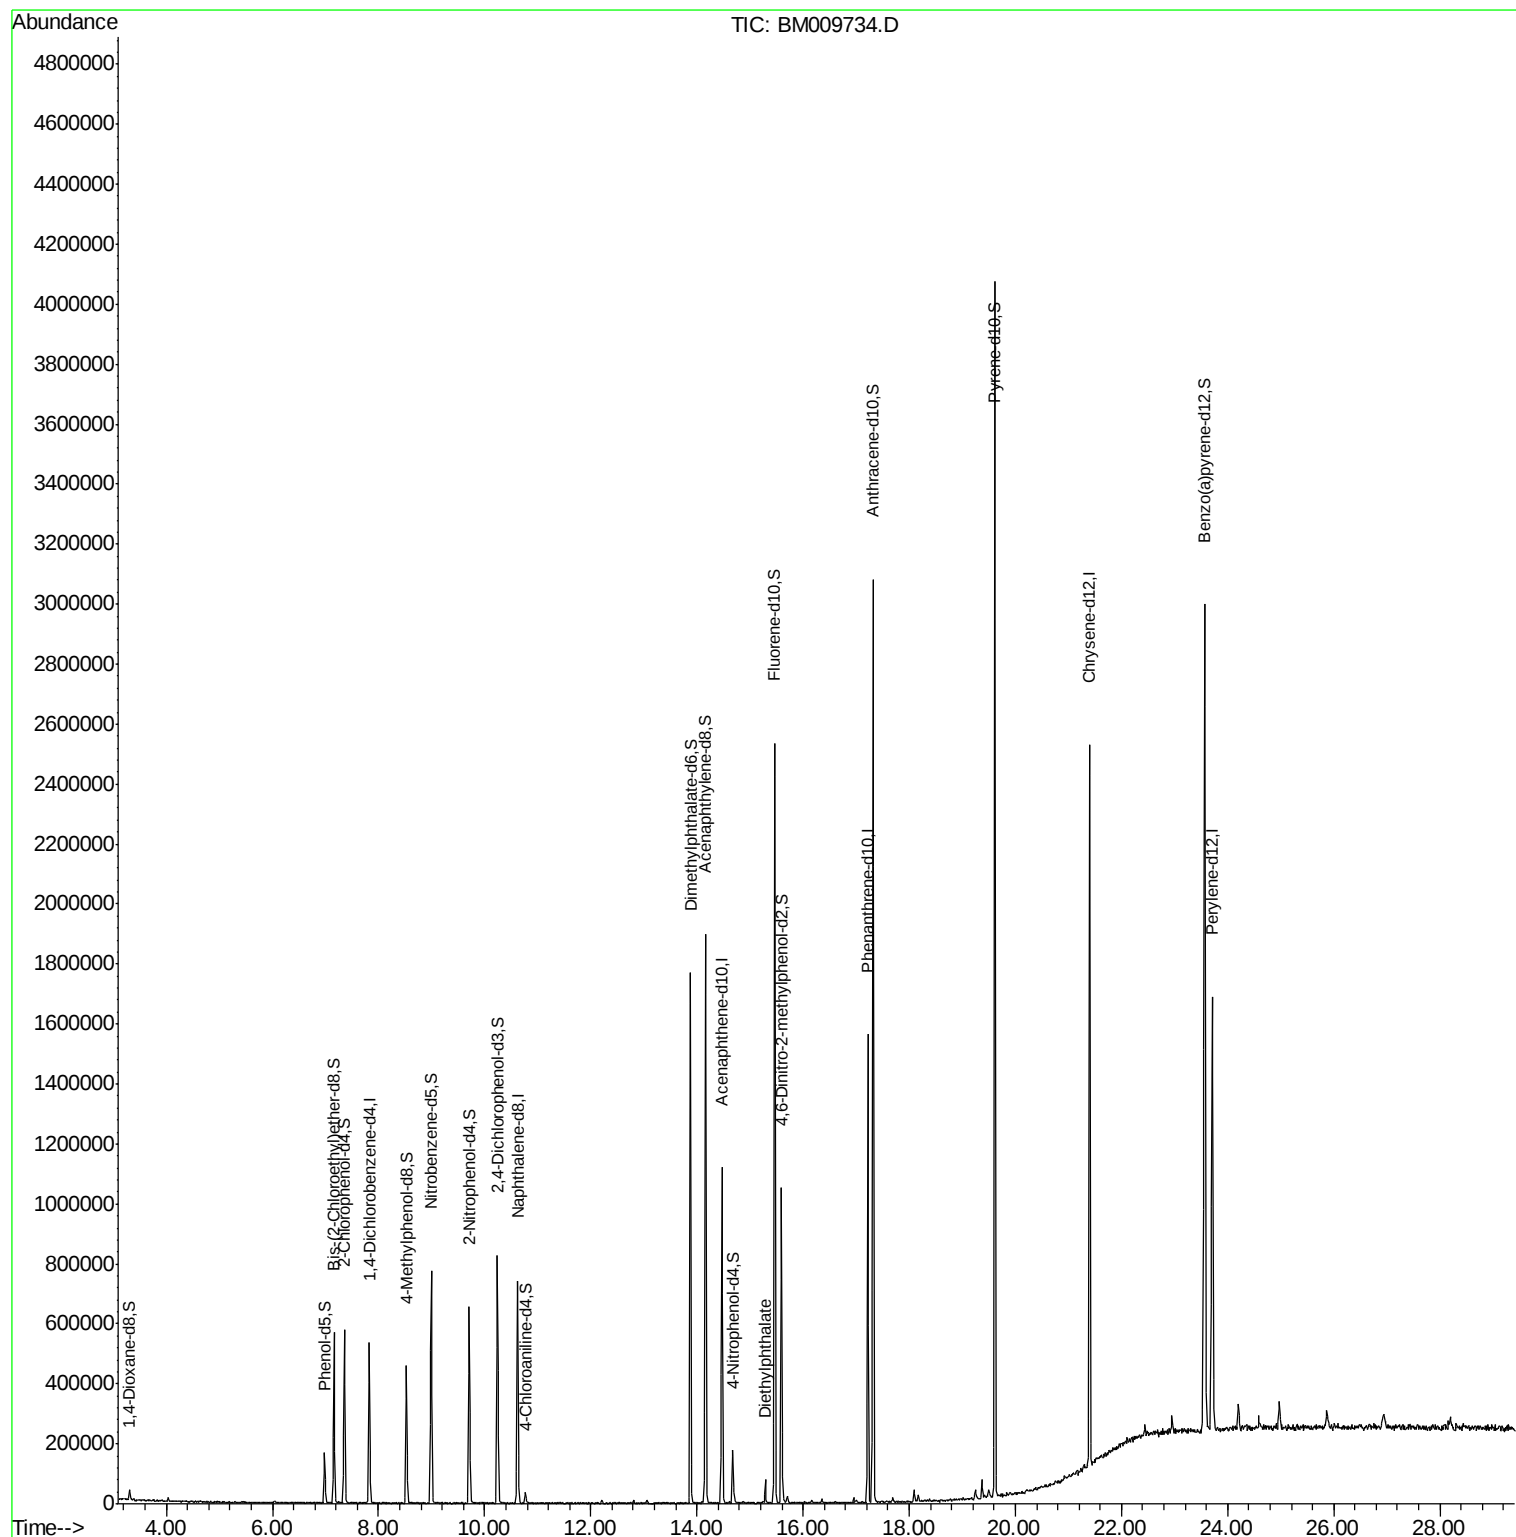


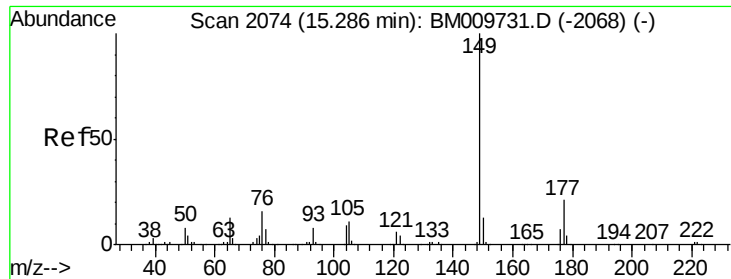

#56
 Diethylphthalate
 Concen: 1.16 ng/ul
 RT: 15.29 min Scan# 2074
 Delta R.T. -0.00 min
 Lab File: BM009734.D
 Acq: 27 Apr 2017 10:51

Instrument :
 BNA_M
 ClientSampleId :
 JHTC1

Tgt Ion:149 Resp: 36280
 Ion Ratio Lower Upper
 149 100
 177 20.3 17.3 25.9
 150 10.0 11.0 16.6#

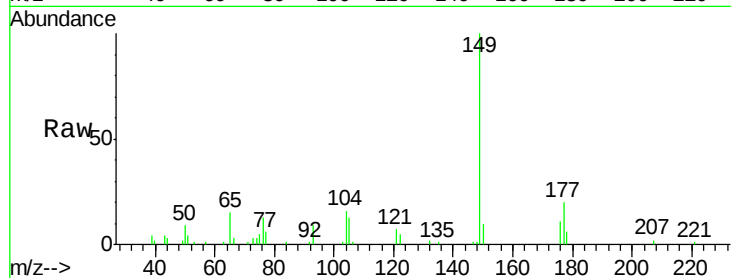

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 177.00 (176.70 to 177.70): E
 Ion 150.00 (149.70 to 150.70): E

