

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009743.D
 Acq On : 27 Apr 2017 16:50
 Operator : SJ/MA
 Sample : I2809-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHTD5

Quant Time: Apr 27 18:34:36 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Apr 27 18:07:34 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	153970	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	694947	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	442748	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1088200	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1386260	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	1097369	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.31	96	18834	5.63	ng/uL	0.00
5) Phenol-d5	6.99	99	113984	6.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	328589	28.81	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	265870	24.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	212183	16.27	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	169035	29.88	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	194199	32.63	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	346520	29.11	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	11379	0.79	ng/ul	0.01
43) Dimethylphthalate-d6	13.88	166	1269082	32.95	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1533362	33.01	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	44024	5.92	ng/ul	0.00
57) Fluorene-d10	15.46	176	1155204	33.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	216794	28.24	ng/ul	0.00
70) Anthracene-d10	17.32	188	1940502	34.73	ng/ul	0.00
76) Pyrene-d10	19.62	212	2293792	37.49	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1843903	34.55	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	201827	5.30	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009743.D
Acq On : 27 Apr 2017 16:50
Operator : SJ/MA
Sample : I2809-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHTD5

Quant Time: Apr 27 18:34:36 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Apr 27 18:07:34 2017
Response via : Initial Calibration

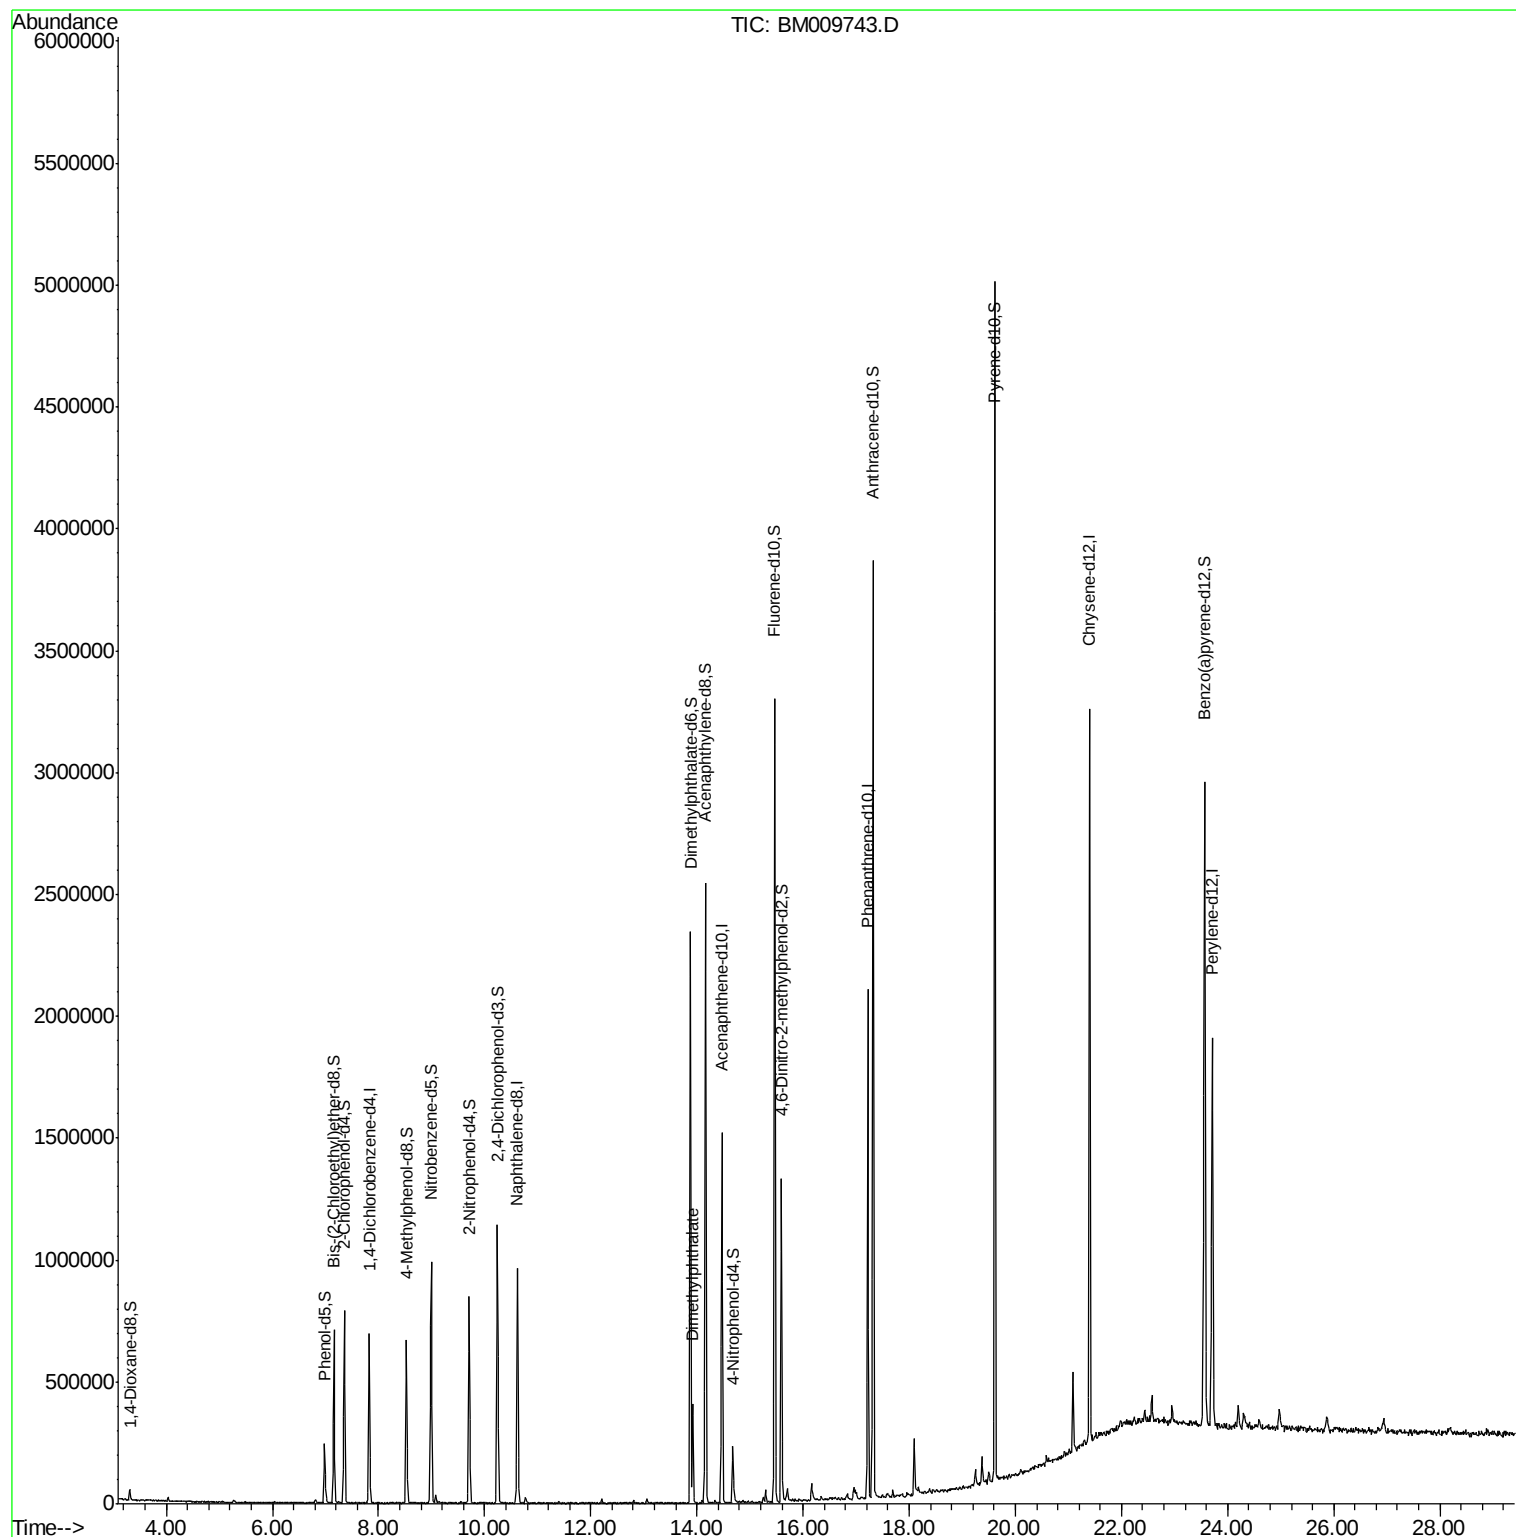

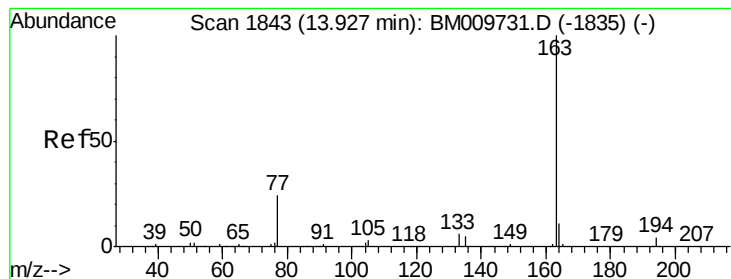

#44
 Dimethylphthalate
 Concen: 5.30 ng/ul
 RT: 13.92 min Scan# 1842
 Delta R.T. -0.01 min
 Lab File: BM009743.D
 Acq: 27 Apr 2017 16:50

Instrument :
 BNA_M
 ClientSampleId :
 JHTD5

Tgt Ion:	163	Resp:	201827
Ion	Ratio	Lower	Upper
163	100		
194	3.7	3.0	4.6
164	9.9	8.6	12.8

