

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009756.D
 Acq On : 28 Apr 2017 00:41
 Operator : SJ/MA
 Sample : I2806-01
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSM0

Quant Time: Apr 28 01:25:15 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 01:10:39 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	127033	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	498229	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	282303	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	656790	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	910970	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	830809	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	11505	4.17	ng/uL	0.00
5) Phenol-d5	6.99	99	266632	19.32	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	188339	20.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.36	132	184385	21.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	201738	18.75	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	87175	21.50	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	92023	21.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	180302	21.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	127099	12.36	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	577171	23.50	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	702502	23.72	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	101410	21.40	ng/ul	0.00
57) Fluorene-d10	15.46	176	533059	24.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	88200	19.03	ng/ul	0.00
70) Anthracene-d10	17.32	188	863472	25.61	ng/ul	0.00
76) Pyrene-d10	19.61	212	1097281	27.29	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	1124576	27.83	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.92	163	114231	4.70 ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009756.D
Acq On : 28 Apr 2017 00:41
Operator : SJ/MA
Sample : I2806-01
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSM0

Quant Time: Apr 28 01:25:15 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 01:10:39 2017
Response via : Initial Calibration

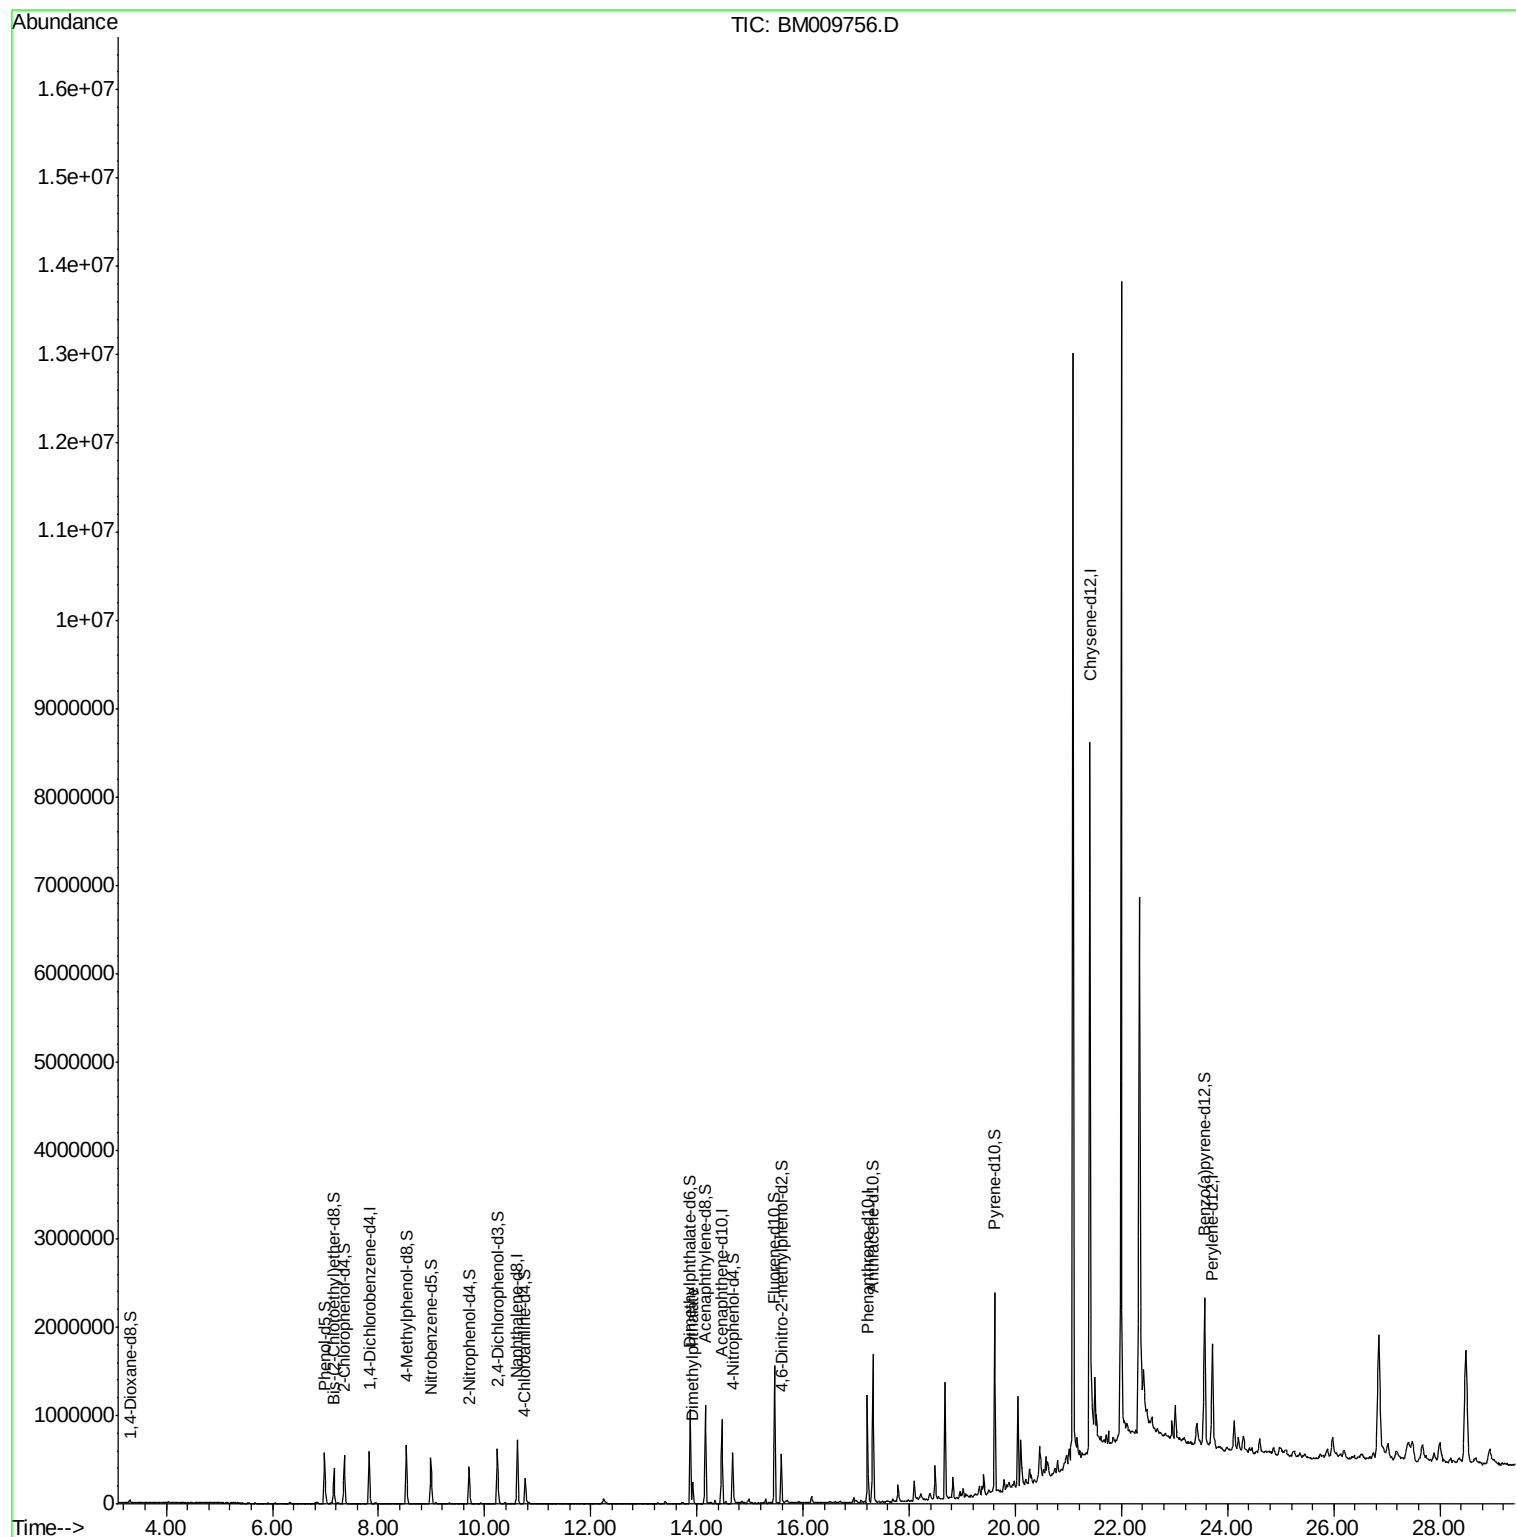

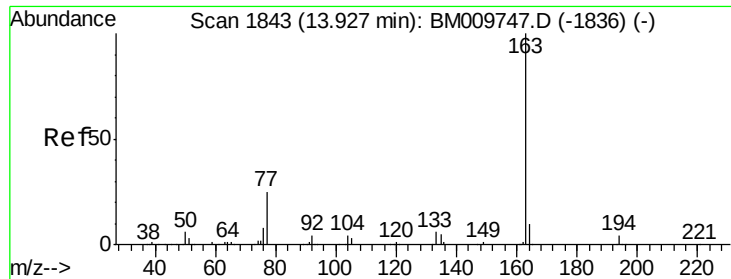

#44

Dimethylphthalate

Concen: 4.70 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BM009756.D

Acq: 28 Apr 2017 00:41

Instrument :

BNA_M

ClientSampleId :

JHSM0


Tgt Ion:163 Resp: 114231

Ion Ratio Lower Upper

163 100

194 3.9 3.0 4.6

164 8.8 8.6 12.8

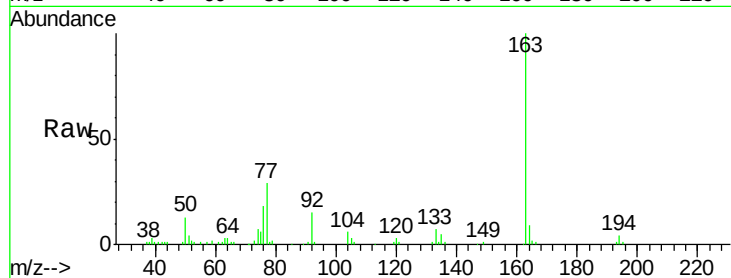

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

