

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009761.D
 Acq On : 28 Apr 2017 03:41
 Operator : SJ/MA
 Sample : I2806-06
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSM5

Quant Time: Apr 28 04:37:11 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 01:10:39 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	181120	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	782848	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	483478	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1159897	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1203539	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	900356	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	23951	6.09	ng/uL	0.00
5) Phenol-d5	6.99	99	600616	30.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	441509	32.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	413762	33.05	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	479618	31.27	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	220771	34.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.71	143	255517	38.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	436139	32.53	ng/ul	0.00
29) 4-Chloroaniline-d4	10.77	131	597642	37.00	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	1462575	34.78	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1847871	36.43	ng/ul	0.00
51) 4-Nitrophenol-d4	14.68	143	269953	33.27	ng/ul	0.00
57) Fluorene-d10	15.46	176	1341826	35.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	248617	30.38	ng/ul	0.00
70) Anthracene-d10	17.32	188	2156249	36.21	ng/ul	0.00
76) Pyrene-d10	19.62	212	2359029	44.41	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1620307	37.00	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.92	163	353503	8.50	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009761.D
Acq On : 28 Apr 2017 03:41
Operator : SJ/MA
Sample : I2806-06
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSM5

Quant Time: Apr 28 04:37:11 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 01:10:39 2017
Response via : Initial Calibration

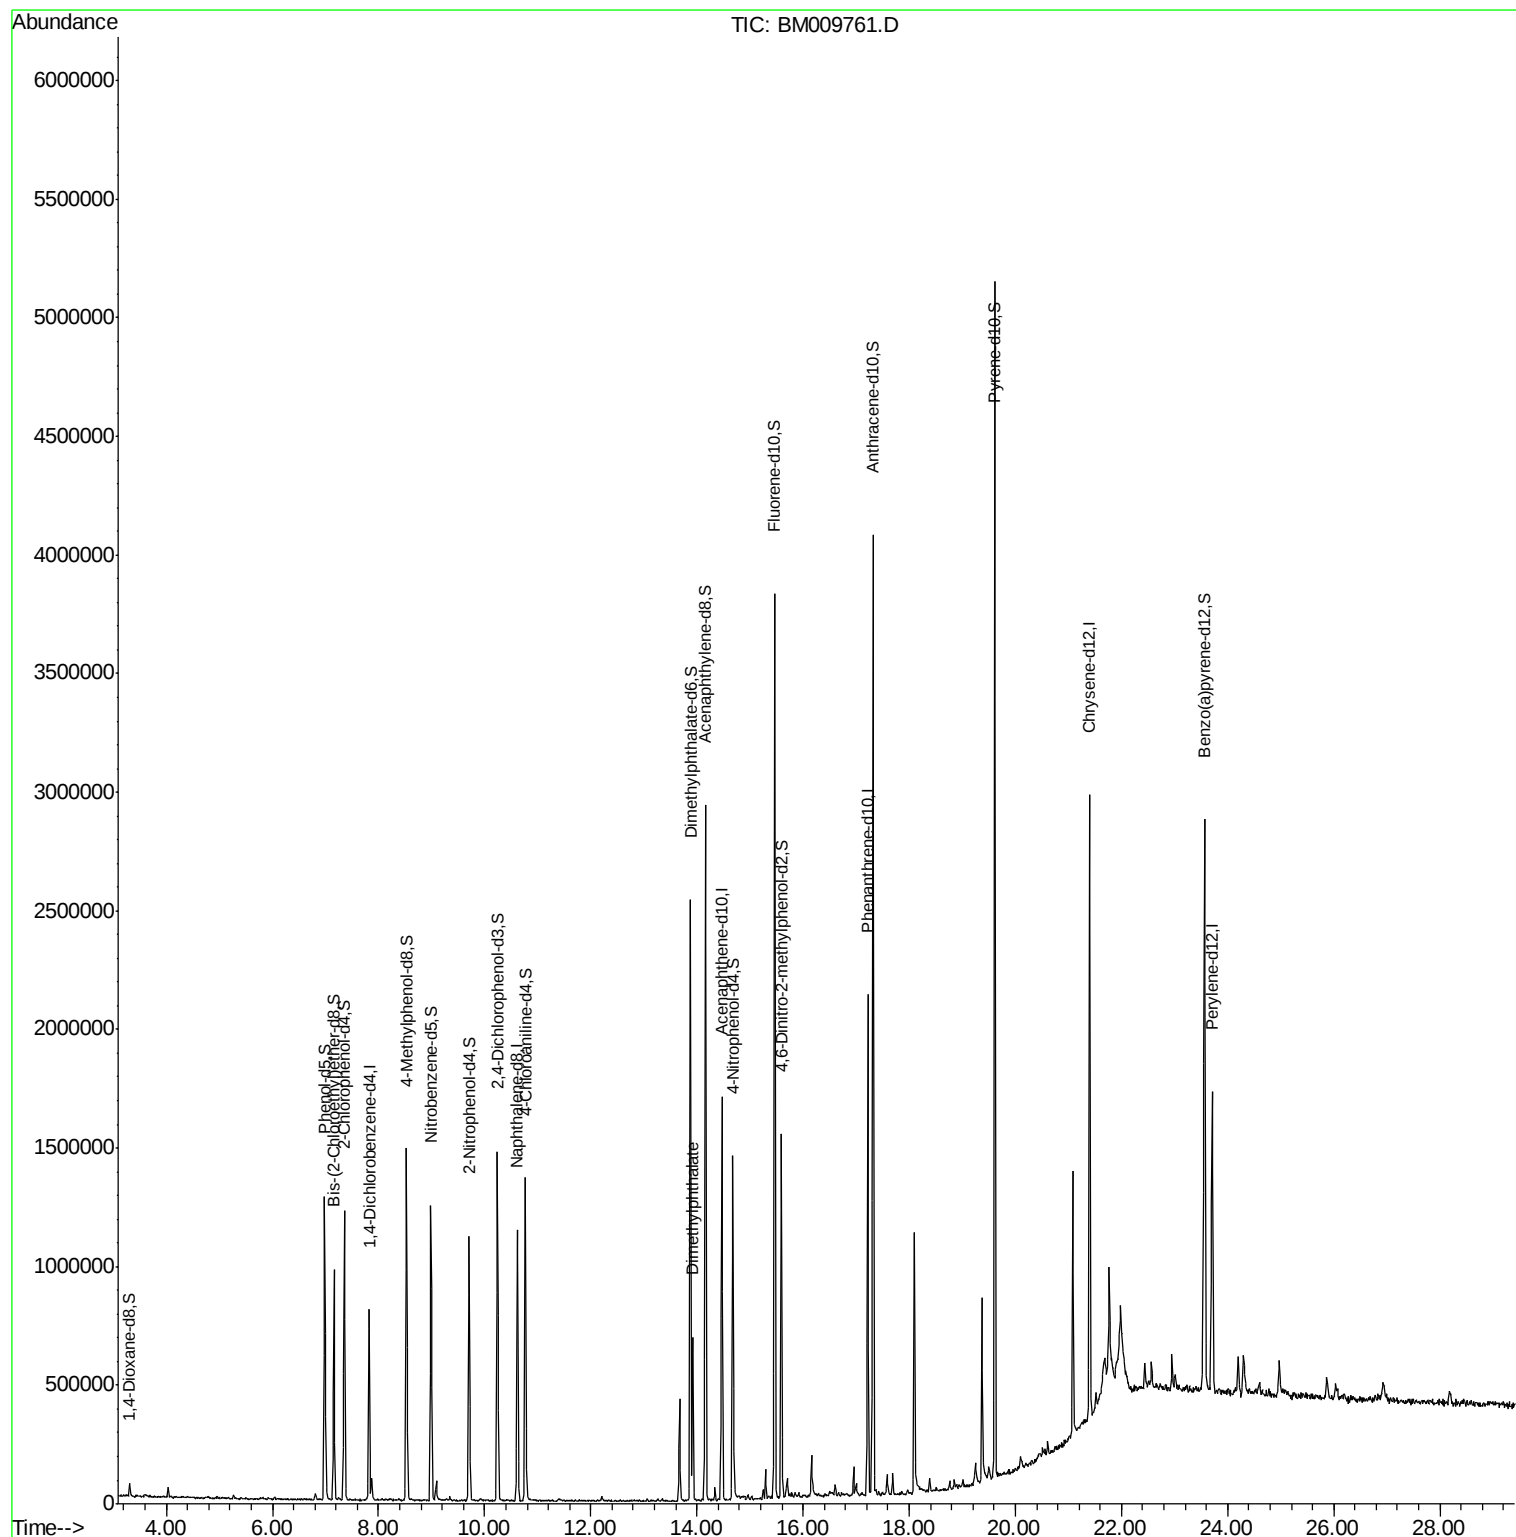


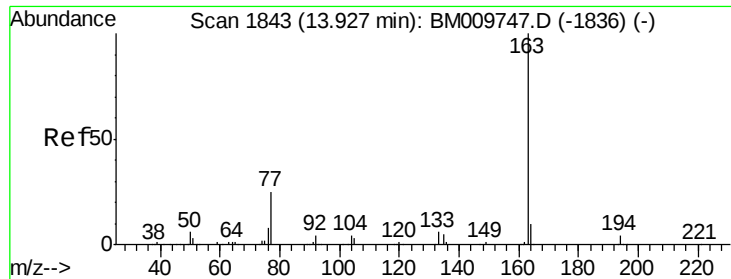

#44
 Dimethylphthalate
 Concen: 8.50 ng/ul
 RT: 13.92 min Scan# 1842
 Delta R.T. -0.01 min
 Lab File: BM009761.D
 Acq: 28 Apr 2017 03:41

Instrument :
 BNA_M
 ClientSampleId :
 JHSM5

Tgt Ion:163 Resp: 353503
 Ion Ratio Lower Upper
 163 100
 194 4.1 3.0 4.6
 164 10.8 8.6 12.8

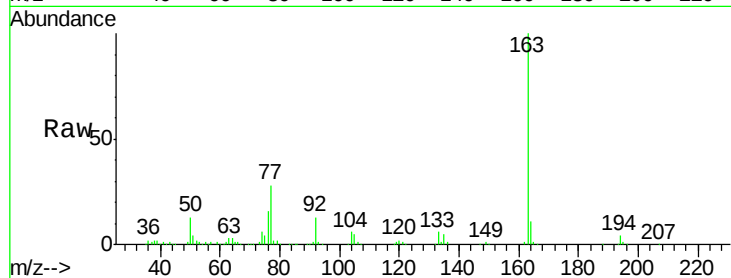

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

