

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009765.D
 Acq On : 28 Apr 2017 06:04
 Operator : SJ/MA
 Sample : I2806-09
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSN2

Quant Time: Apr 28 06:37:16 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 06:36:45 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	148562	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	650081	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	427603	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1090707	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1385219	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	1142118	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	9917	3.07	ng/uL	0.00
5) Phenol-d5	6.99	99	262231	16.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	192551	17.50	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	179223	17.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	209006	16.61	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	93196	17.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	106008	19.04	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	193922	17.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	211467	15.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	712304	19.15	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	870860	19.41	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	120852	16.84	ng/ul	0.00
57) Fluorene-d10	15.46	176	659315	19.64	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	106979	13.90	ng/ul	0.00
70) Anthracene-d10	17.32	188	1100161	19.65	ng/ul	0.00
76) Pyrene-d10	19.61	212	1320639	21.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1133142	20.40	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	123151	3.35	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009765.D
Acq On : 28 Apr 2017 06:04
Operator : SJ/MA
Sample : I2806-09
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSN2

Quant Time: Apr 28 06:37:16 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 06:36:45 2017
Response via : Initial Calibration

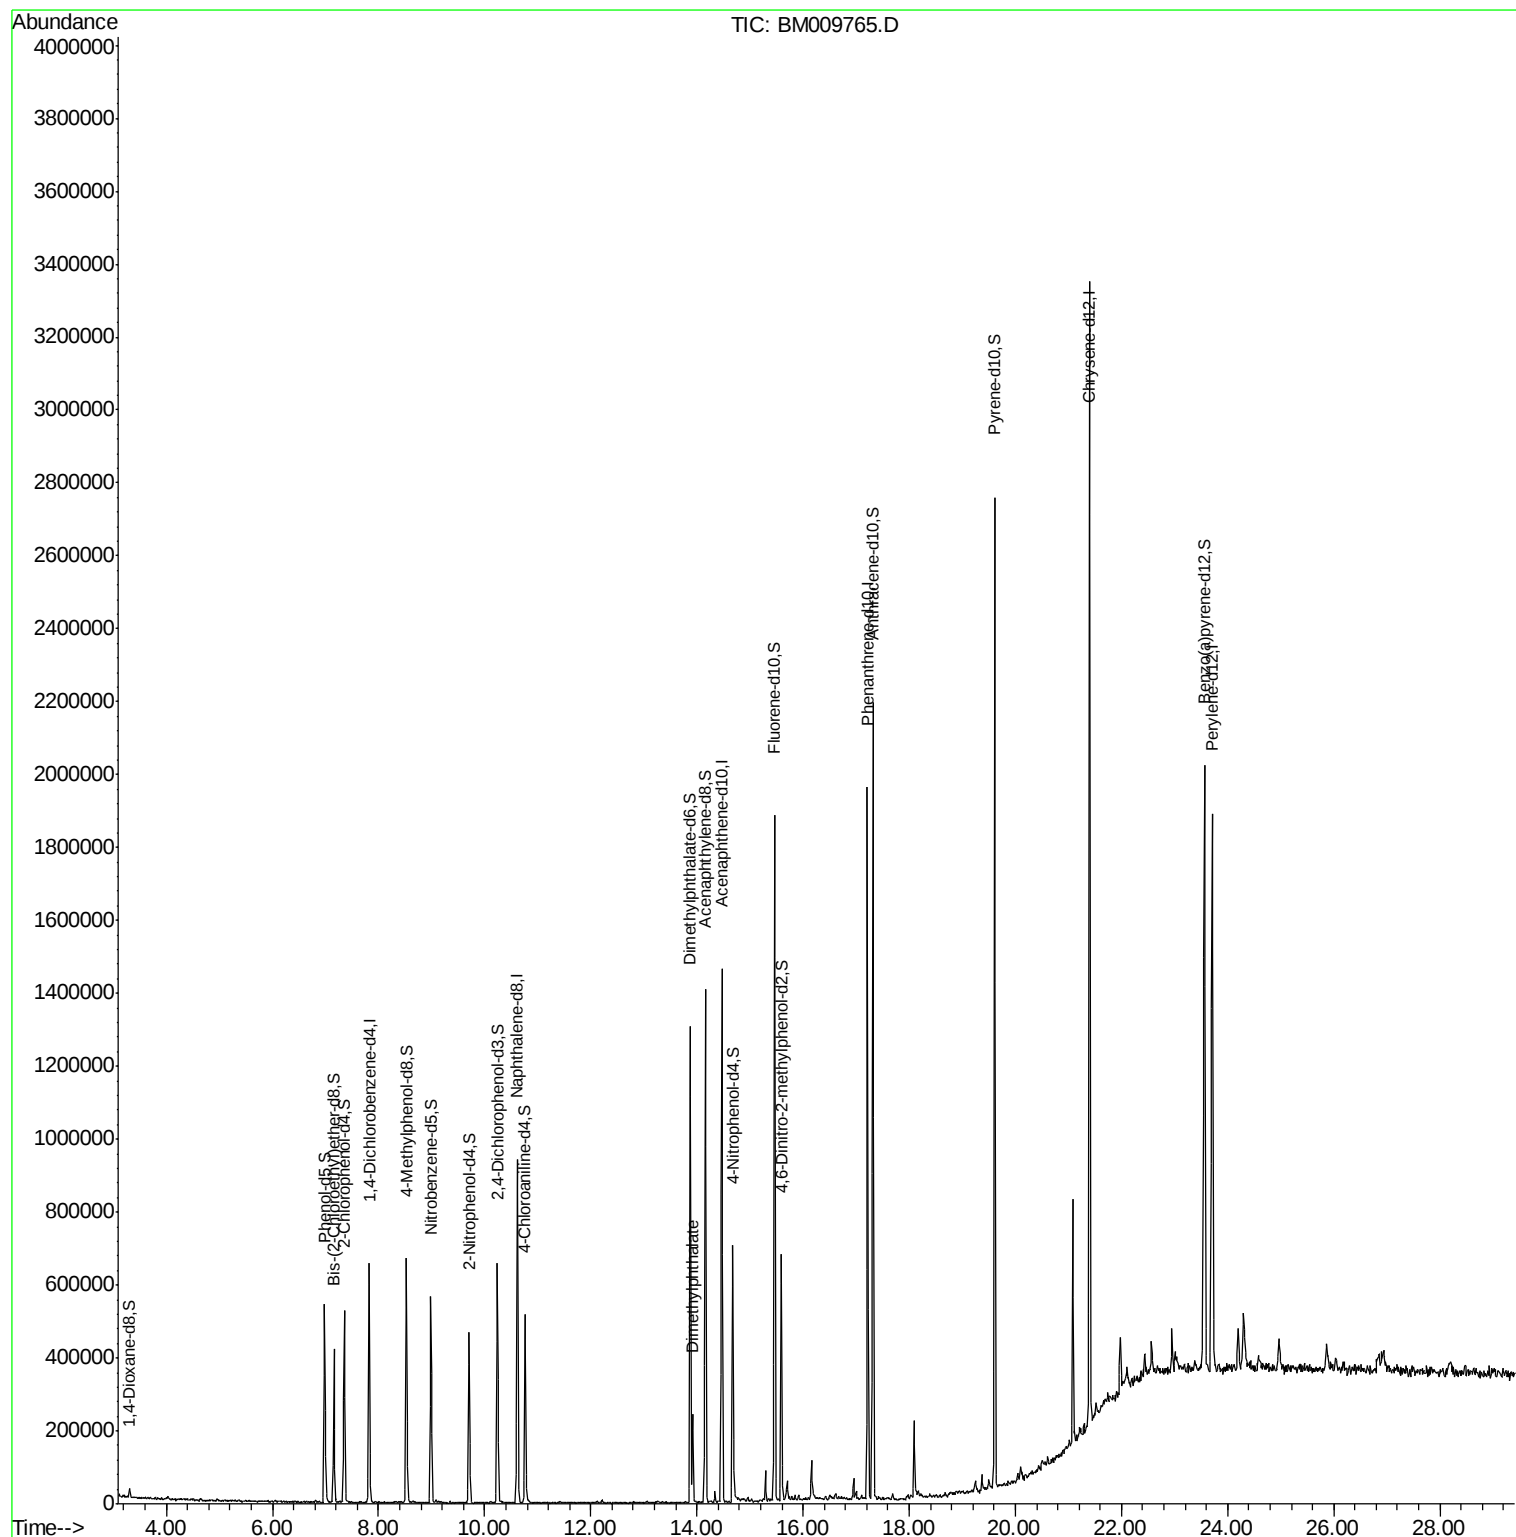

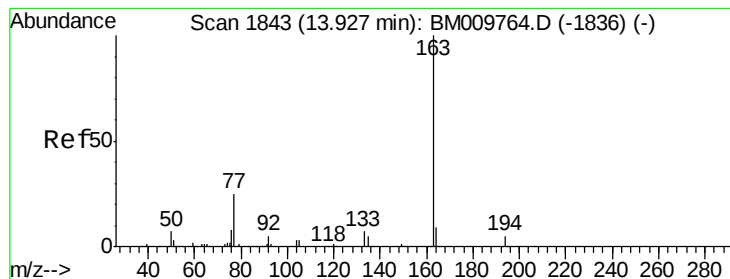

#44

Dimethylphthalate

Concen: 3.35 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BM009765.D

Acq: 28 Apr 2017 06:04

Instrument :

BNA_M

ClientSampleId :

JHSN2


Tgt Ion:163 Resp: 123151

Ion Ratio Lower Upper

163 100

194 4.1 3.0 4.6

164 11.5 8.6 12.8

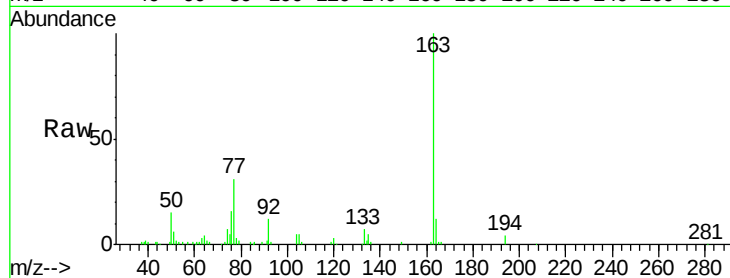

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

