

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009766.D
 Acq On : 28 Apr 2017 06:40
 Operator : SJ/MA
 Sample : I2806-10
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSN3

Quant Time: Apr 28 07:58:33 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 06:36:45 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	144374	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	653660	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	440067	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1100508	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1461318	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	1232436	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	16091	5.13	ng/uL	0.00
5) Phenol-d5	6.99	99	446801	28.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	326716	30.55	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	300928	30.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	368516	30.14	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	167566	31.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	191005	34.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	345992	30.91	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	465554	34.51	ng/ul	0.00
43) Dimethylphthalate-d6	13.88	166	1297533	33.89	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1566225	33.92	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	237423	32.14	ng/ul	0.00
57) Fluorene-d10	15.46	176	1194958	34.58	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	231375	29.80	ng/ul	0.00
70) Anthracene-d10	17.32	188	2044969	36.19	ng/ul	0.00
76) Pyrene-d10	19.62	212	2416989	37.48	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	2202542	36.75	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	251363	6.64	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009766.D
Acq On : 28 Apr 2017 06:40
Operator : SJ/MA
Sample : I2806-10
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSN3

Quant Time: Apr 28 07:58:33 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 06:36:45 2017
Response via : Initial Calibration

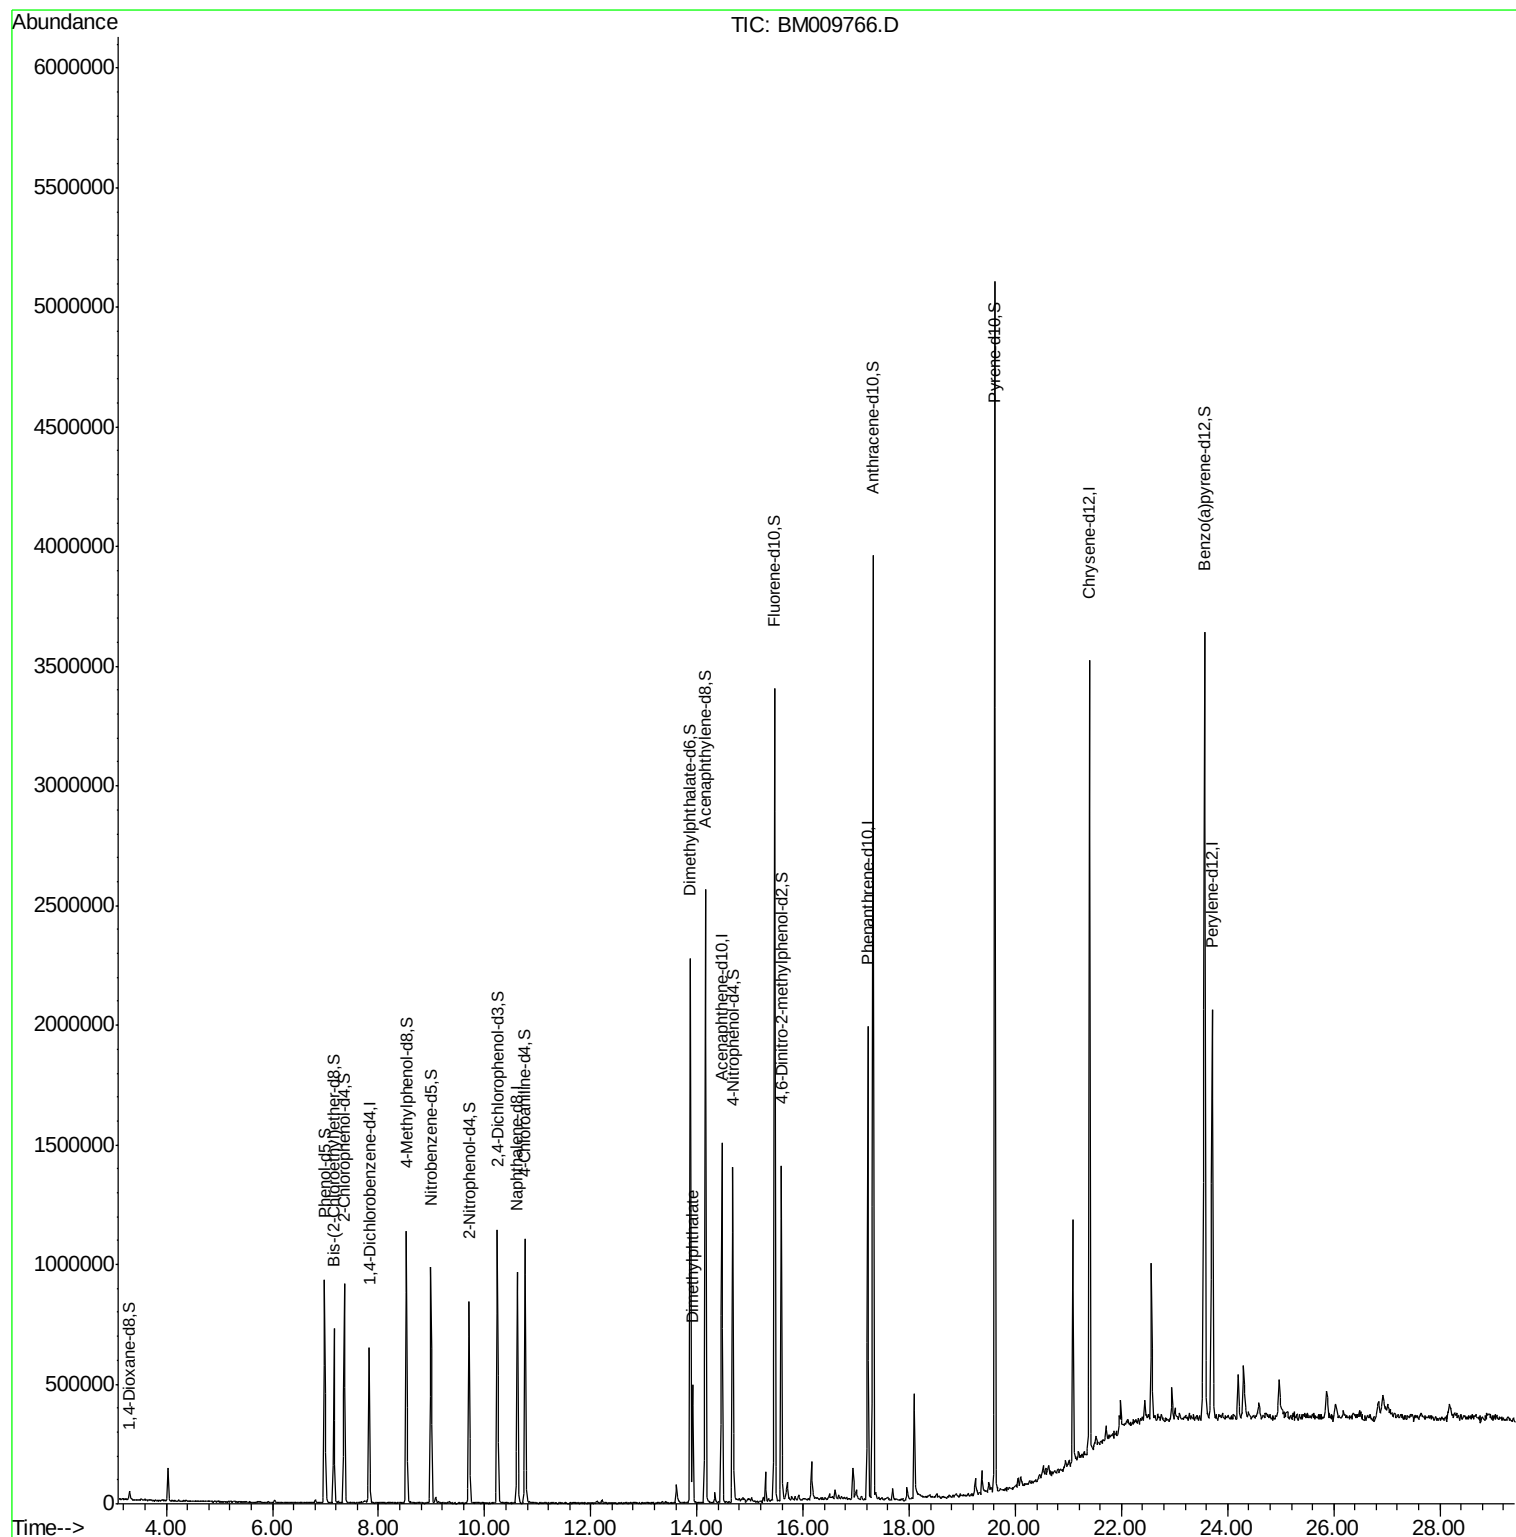

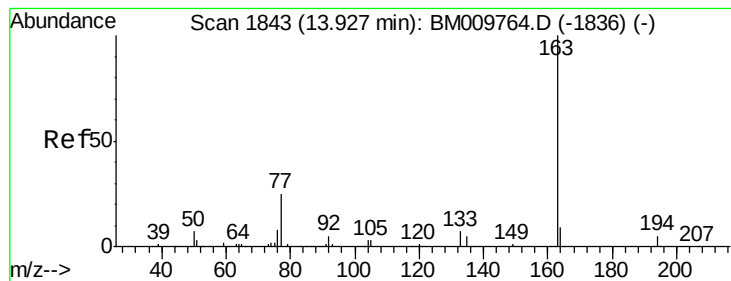

#44

Dimethylphthalate

Concen: 6.64 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BM009766.D

Acq: 28 Apr 2017 06:40

Instrument :

BNA_M

ClientSampleId :

JHSN3


Tgt Ion:163 Resp: 251363

Ion Ratio Lower Upper

163 100

194 4.2 3.0 4.6

164 9.1 8.6 12.8

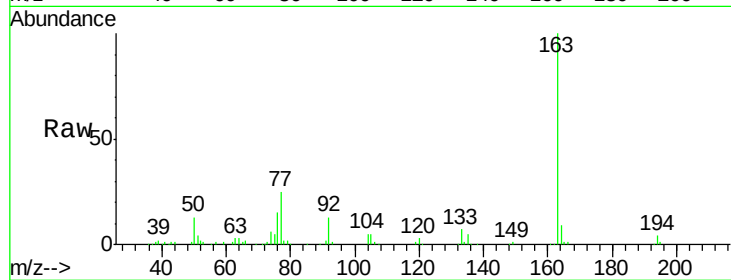

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

