

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009771.D
 Acq On : 28 Apr 2017 09:40
 Operator : SJ/MA
 Sample : I2806-16
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHT18

Quant Time: Apr 28 11:40:14 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 06:36:45 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	142705	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	619726	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	390514	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	972370	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1347882	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	1134865	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	8122	2.62	ng/uL	0.00
5) Phenol-d5	6.99	99	245982	15.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	173257	16.39	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	166896	16.92	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	196540	16.26	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	87086	17.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	91584	17.26	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	185507	17.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	197101	15.41	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	567344	16.70	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	739609	18.05	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	85864	13.10	ng/ul	0.00
57) Fluorene-d10	15.46	176	555737	18.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	79917	11.65	ng/ul	0.00
70) Anthracene-d10	17.32	188	932575	18.68	ng/ul	0.00
76) Pyrene-d10	19.61	212	1159907	19.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1057755	19.16	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.92	163	145223	4.32 ng/ul#	98




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009771.D
Acq On : 28 Apr 2017 09:40
Operator : SJ/MA
Sample : I2806-16
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHT18

Quant Time: Apr 28 11:40:14 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 06:36:45 2017
Response via : Initial Calibration

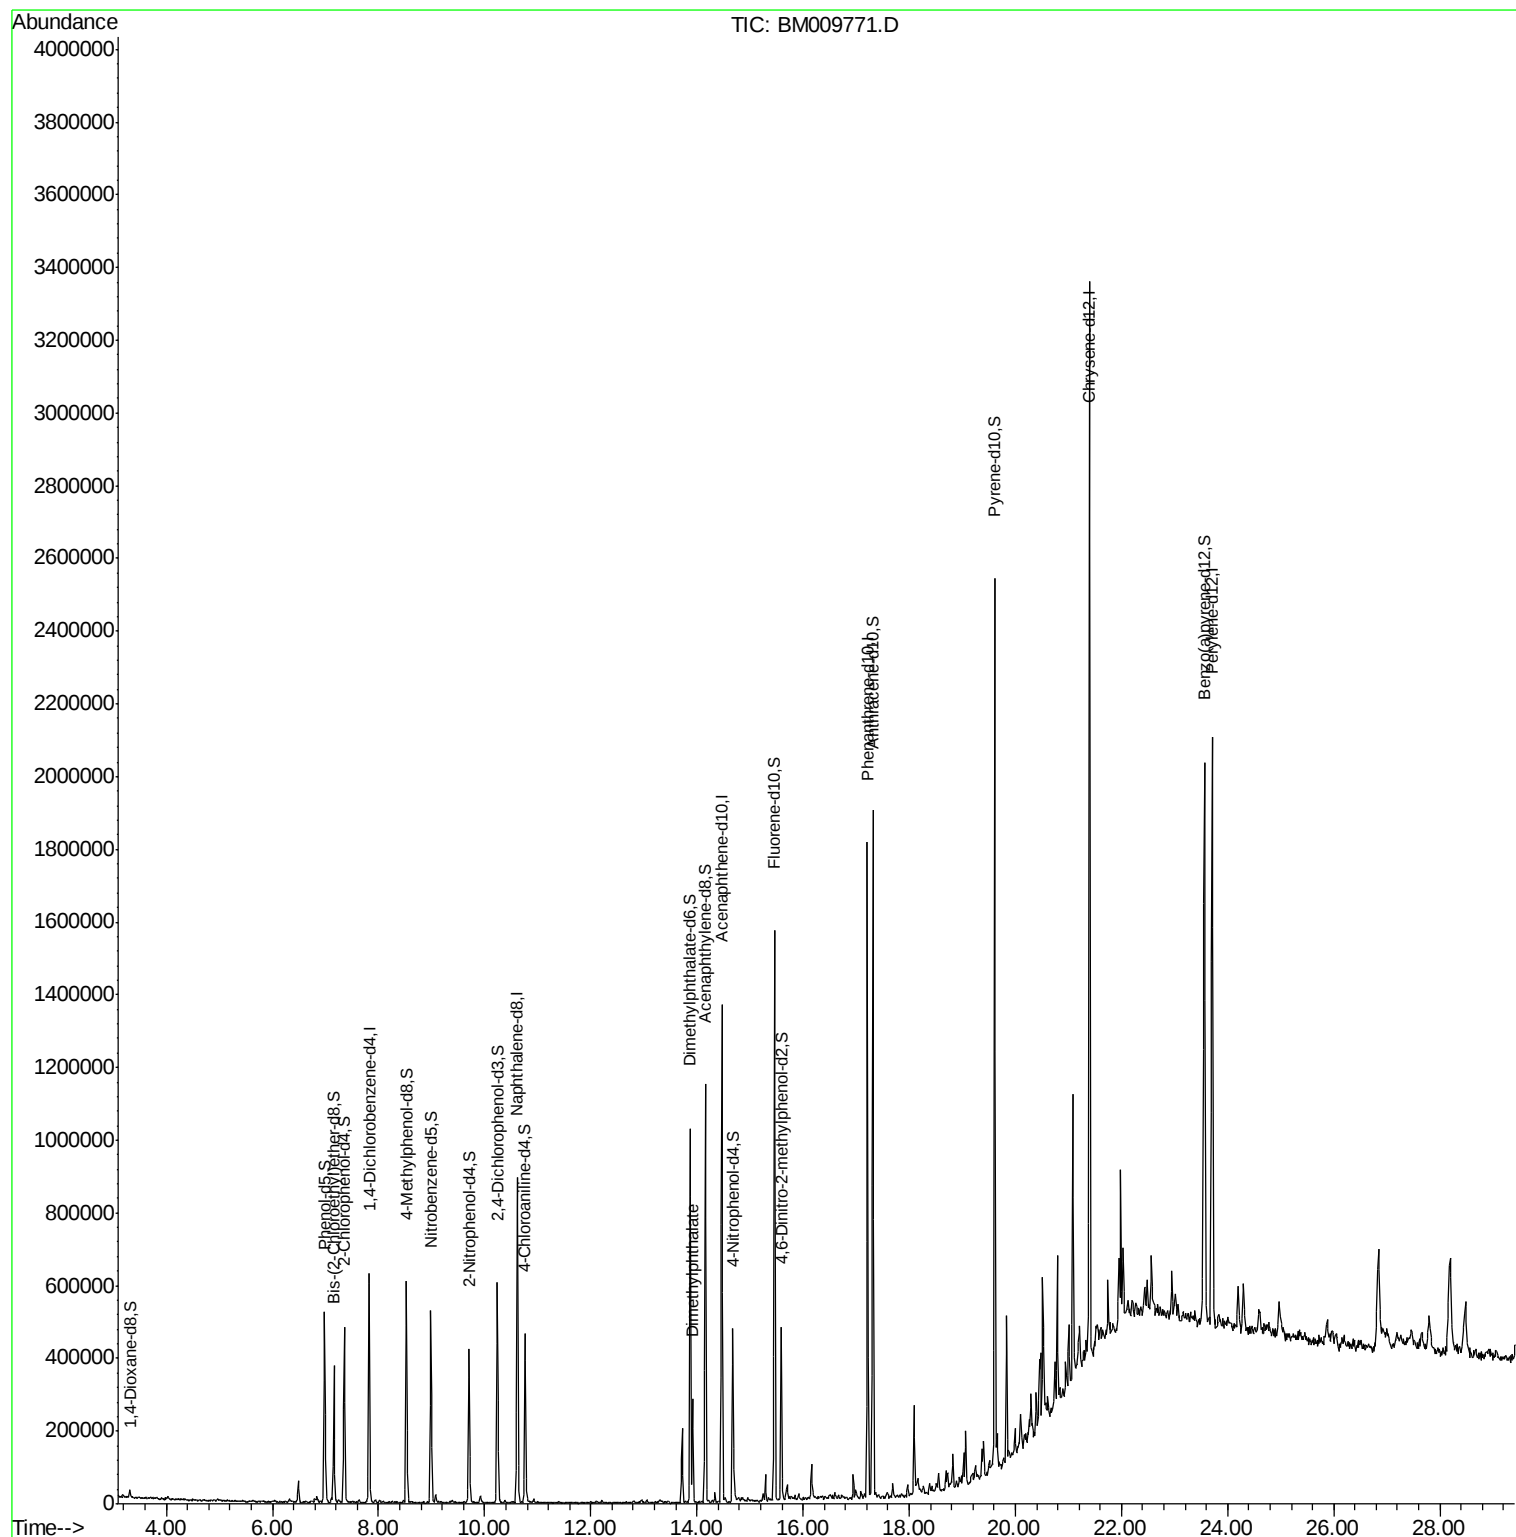

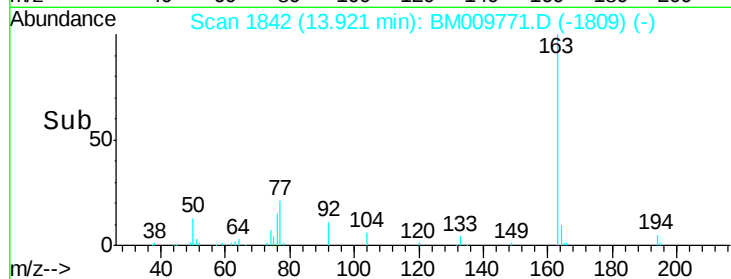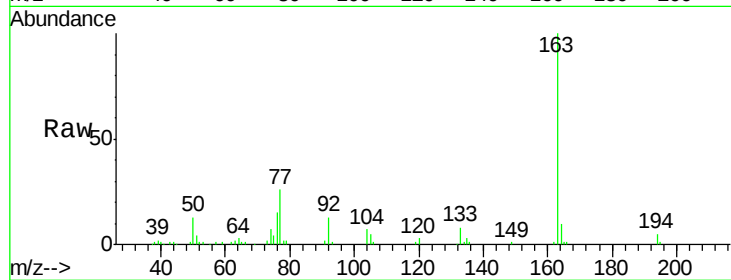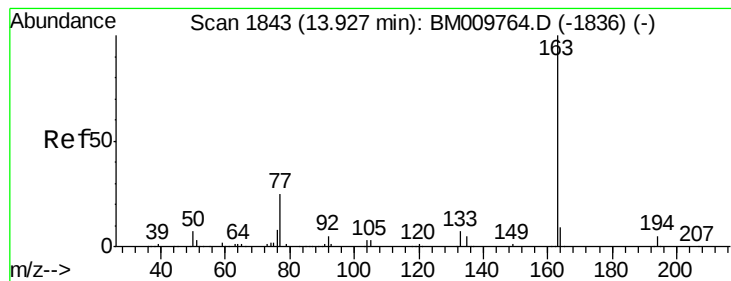

#44

Dimethylphthalate

Concen: 4.32 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BM009771.D

Acq: 28 Apr 2017 09:40

Instrument :

BNA_M

ClientSampleId :

JHT18

Tgt Ion:163 Resp: 145223

Ion Ratio Lower Upper

163 100

194 4.6 3.0 4.6#

164 10.3 8.6 12.8

