

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009772.D
 Acq On : 28 Apr 2017 10:16
 Operator : SJ/MA
 Sample : I2806-17
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHT23

Quant Time: Apr 28 11:47:35 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 06:36:45 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	134836	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	608275	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	400475	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	983426	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1241576	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	992548	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	12863	4.39	ng/uL	0.00
5) Phenol-d5	6.99	99	307719	21.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	216653	21.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	205649	22.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	230472	20.18	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	103842	20.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	117285	22.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	232746	22.34	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	266873	21.26	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	741092	21.27	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	900962	21.44	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	104479	15.54	ng/ul	0.00
57) Fluorene-d10	15.46	176	677227	21.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	93086	13.42	ng/ul	0.00
70) Anthracene-d10	17.32	188	1106464	21.91	ng/ul	0.00
76) Pyrene-d10	19.61	212	1287387	23.49	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1056844	21.89	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.92	163	191661	5.56	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009772.D
Acq On : 28 Apr 2017 10:16
Operator : SJ/MA
Sample : I2806-17
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHT23

Quant Time: Apr 28 11:47:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 06:36:45 2017
Response via : Initial Calibration

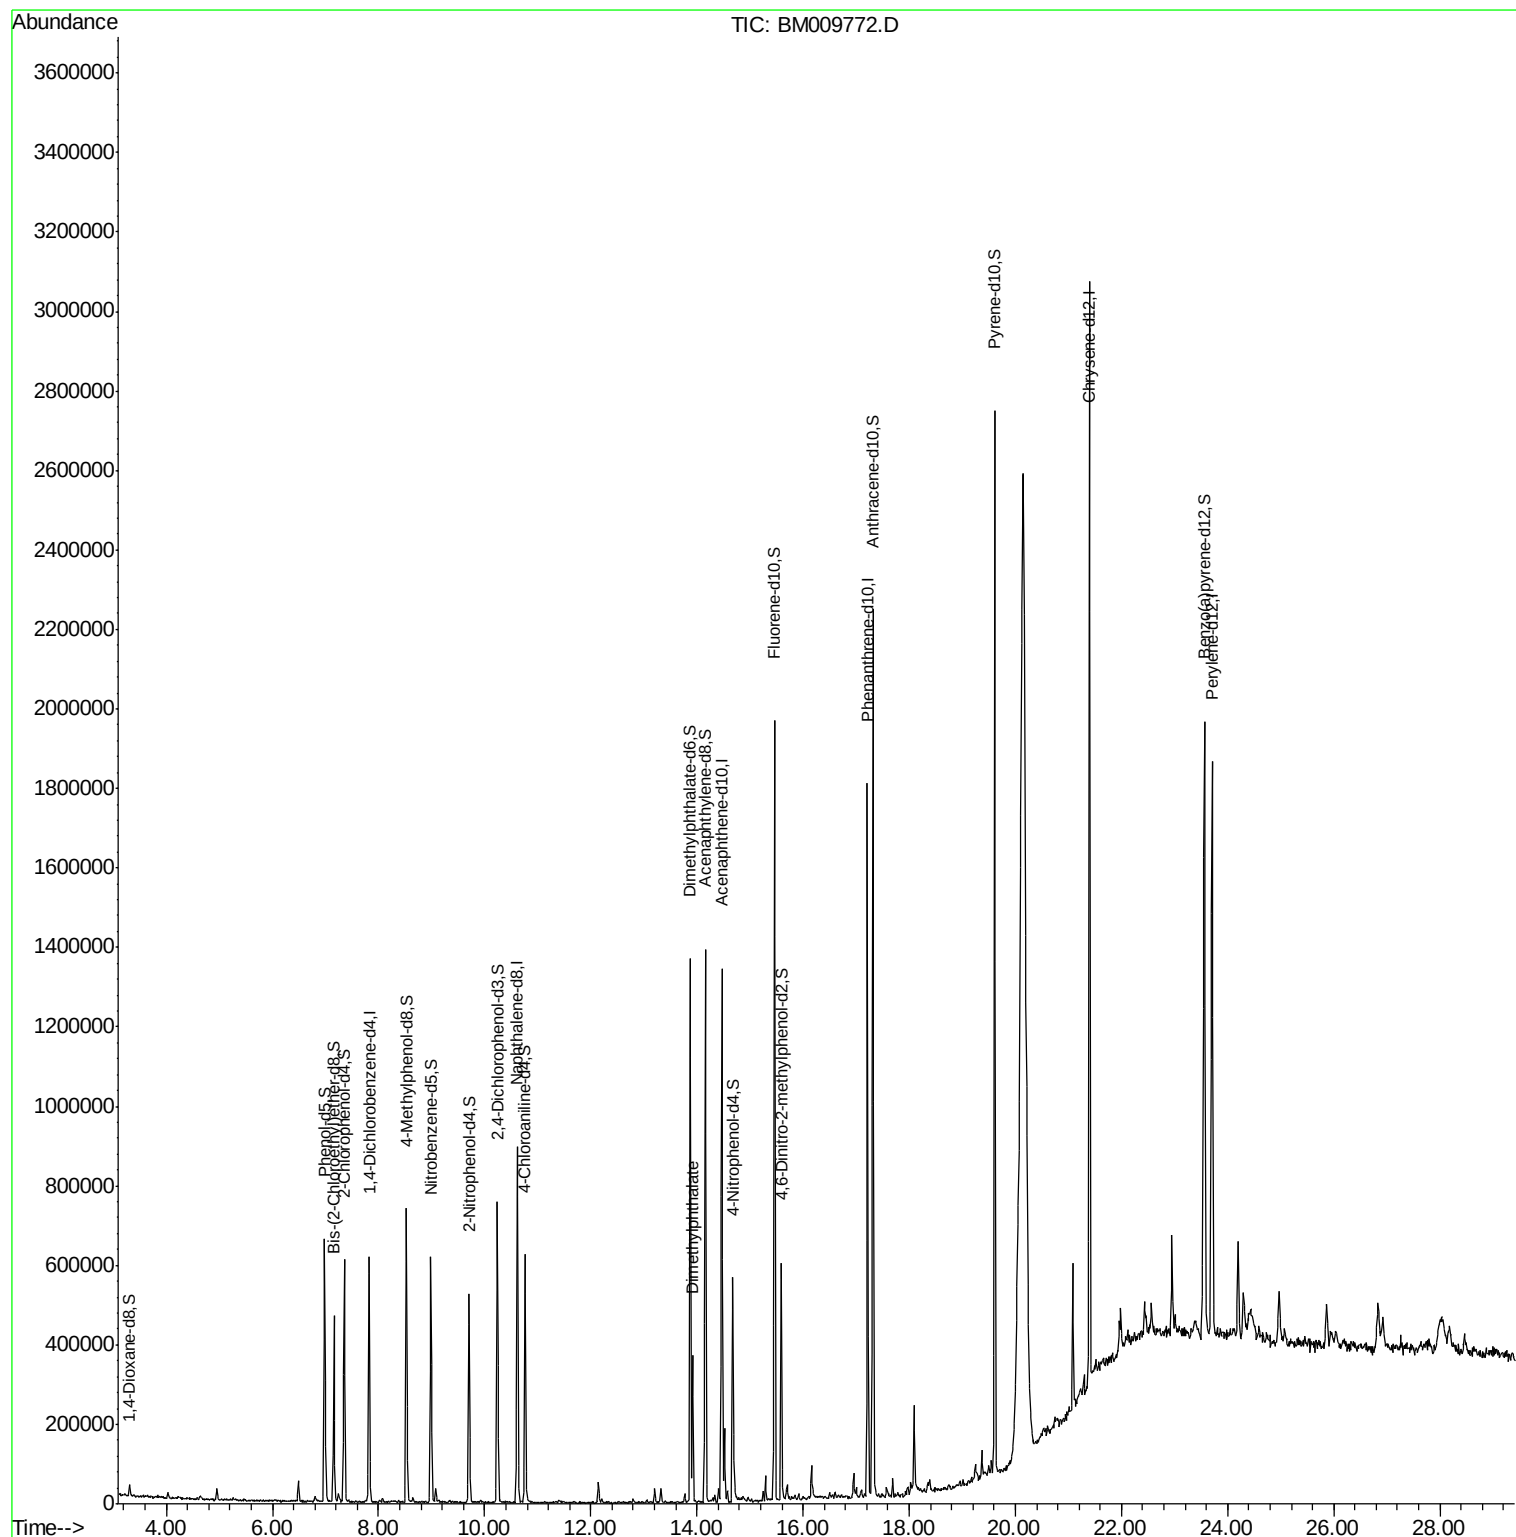

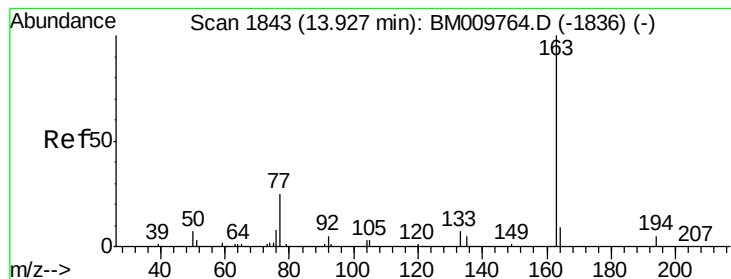

#44

Dimethylphthalate

Concen: 5.56 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BM009772.D

Acq: 28 Apr 2017 10:16

Instrument :

BNA_M

ClientSampleId :

JHT23

Tgt Ion:163 Resp: 191661

Ion Ratio Lower Upper

163 100

194 4.7 3.0 4.6#

164 9.4 8.6 12.8

