

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
 Data File : BM009773.D
 Acq On : 28 Apr 2017 10:52
 Operator : SJ/MA
 Sample : I2806-18
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHT24

Quant Time: Apr 28 11:54:04 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 06:36:45 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	158524	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	687682	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	429891	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1067306	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1244311	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	950408	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.30	96	9571	2.78	ng/uL	0.00
5) Phenol-d5	6.98	99	217855	12.65	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	161601	13.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	152342	13.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	173030	12.89	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	76268	13.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	87441	14.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	160746	13.65	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	202444	14.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	555995	14.87	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	654131	14.50	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	82174	11.39	ng/ul	0.00
57) Fluorene-d10	15.46	176	512005	15.17	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	71764	9.53	ng/ul	0.00
70) Anthracene-d10	17.32	188	832771	15.20	ng/ul	0.00
76) Pyrene-d10	19.61	212	969659	17.66	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	735323	15.91	ng/ul	0.00


Target Compounds					Qvalue
44) Dimethylphthalate	13.92	163	128107	3.46 ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009773.D
Acq On : 28 Apr 2017 10:52
Operator : SJ/MA
Sample : I2806-18
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHT24

Quant Time: Apr 28 11:54:04 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 06:36:45 2017
Response via : Initial Calibration

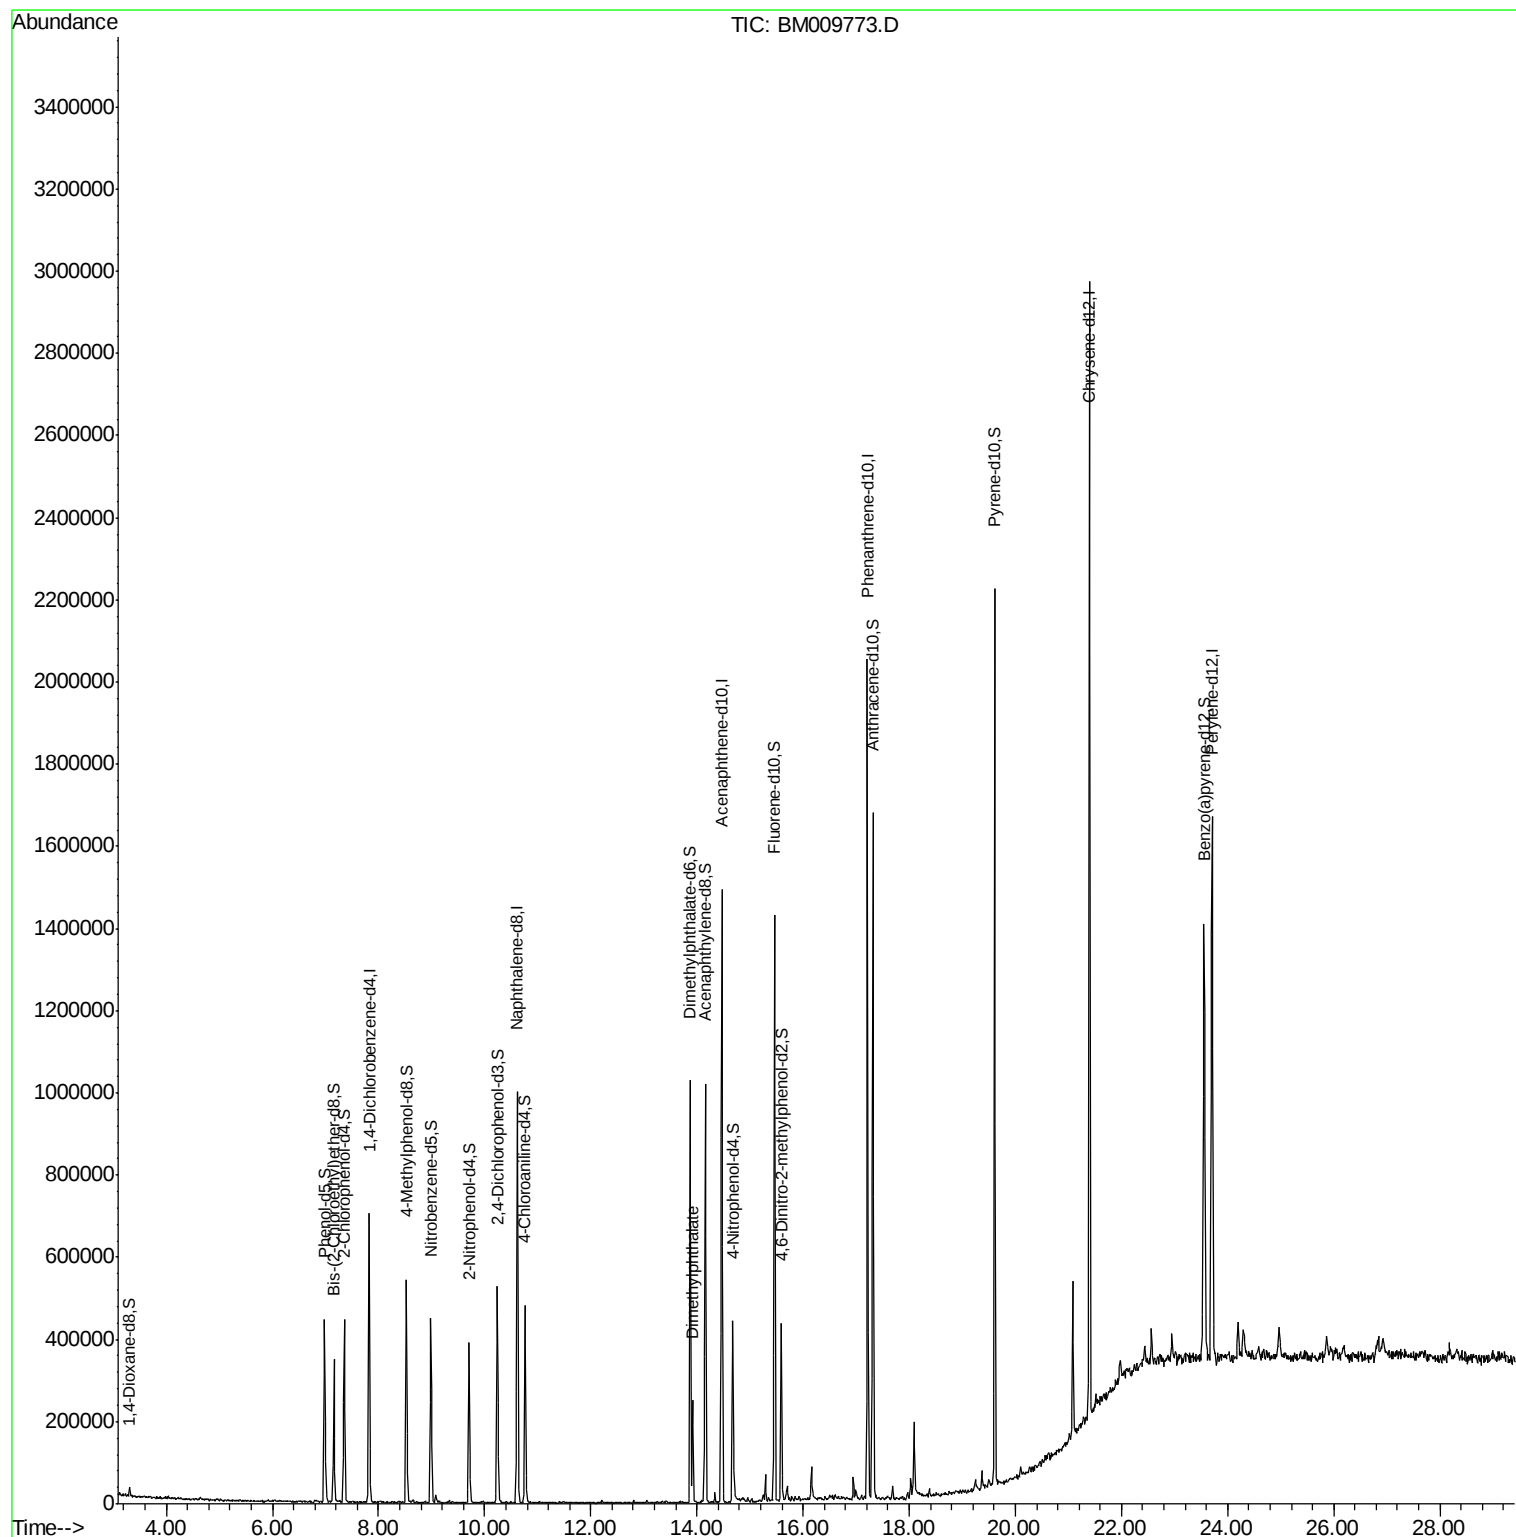

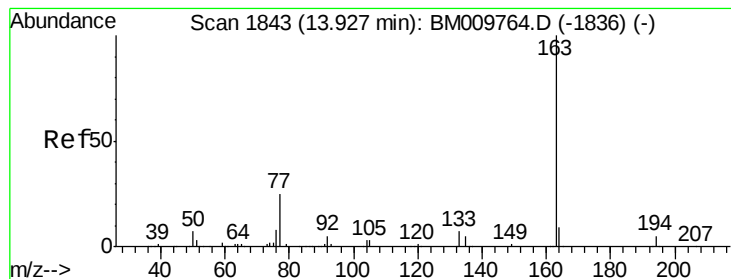

#44

Dimethylphthalate

Concen: 3.46 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.01 min

Lab File: BM009773.D

Acq: 28 Apr 2017 10:52

Instrument :

BNA_M

ClientSampleId :

JHT24


Tgt Ion:163 Resp: 128107

Ion Ratio Lower Upper

163 100

194 5.0 3.0 4.6#

164 10.5 8.6 12.8

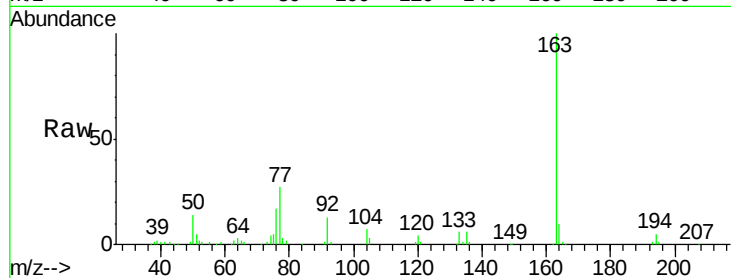

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

