


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042717\
Data File : BM009730.D
Acq On : 27 Apr 2017 08:27
Operator : SJ/MA
Sample : DFTPP07
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP07

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
Title : SVOA CALIBRATION
Last Update : Wed Nov 30 00:32:18 2016

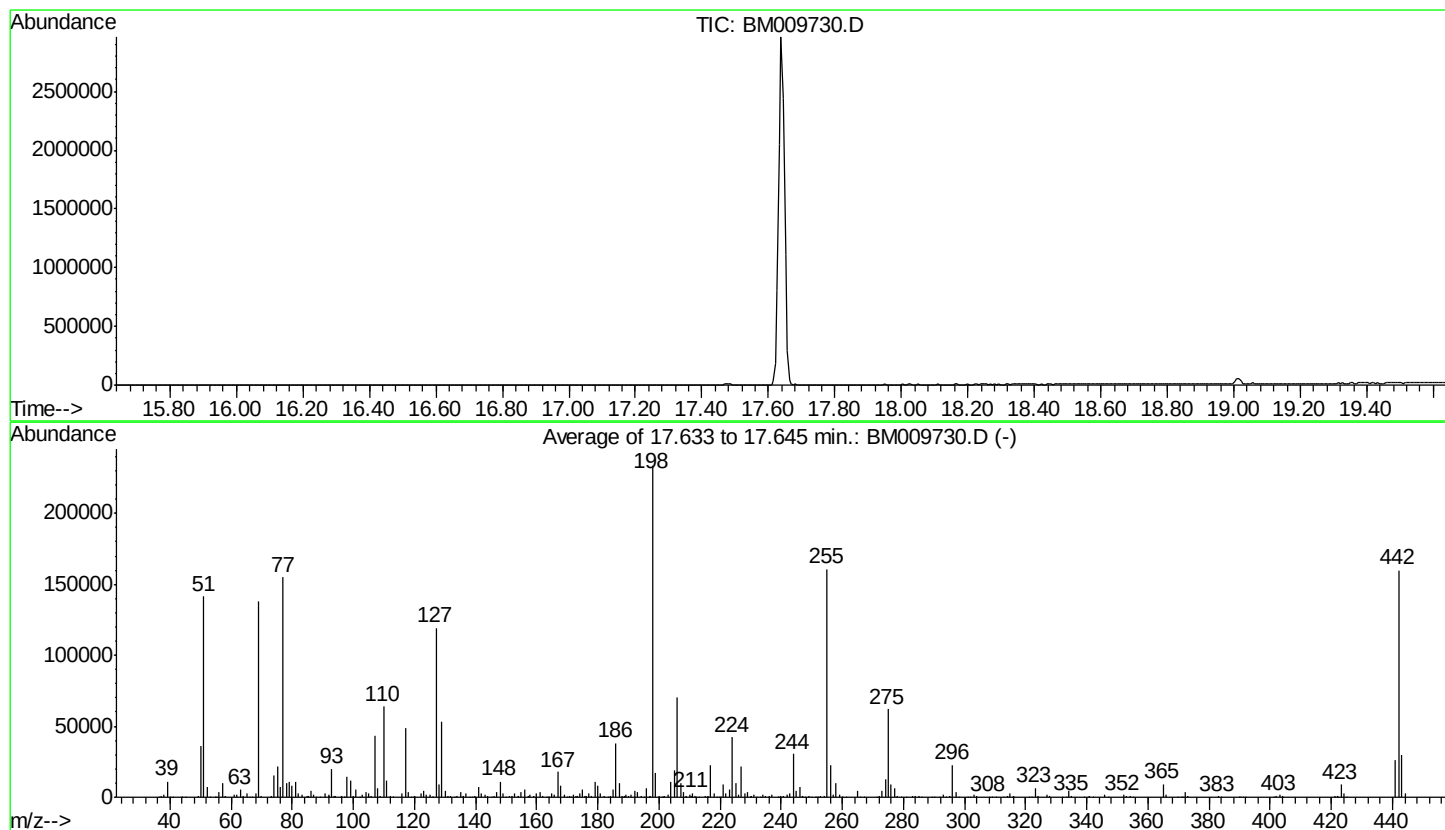

AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.5	141317	PASS
68	69	0.00	2	1.7	2381	PASS
69	198	0.00	100	59.2	138320	PASS
70	69	0.00	2	0.6	852	PASS
127	198	10	80	51.1	119309	PASS
197	198	0.00	2	0.6	1362	PASS
198	198	100	100	100.0	233621	PASS
199	198	5	9	7.2	16936	PASS
275	198	10	60	26.5	61989	PASS
365	198	1	100	4.0	9404	PASS
441	443	0.01	100	87.4	26013	PASS
442	198	50	100	68.5	159960	PASS
443	442	15	24	18.6	29778	PASS

m/z	Abundance
37.00	338.0
38.10	1819.0
39.10	10765.0
40.00	991.0
41.00	538.0
44.00	756.0
49.10	982.0
50.10	33696.0
51.10	136000.0
52.10	7328.0
53.20	437.0
54.90	801.0
56.00	2952.0
57.00	9411.0
58.10	345.0
61.00	1853.0
62.00	2434.0
63.00	5122.0
64.00	813.0
65.10	2417.0
67.00	425.0
68.10	1935.0
69.00	131456.0
69.90	625.0
73.00	1292.0
74.00	14558.0
75.10	19664.0
76.00	8012.0
77.10	142208.0
78.00	10465.0
79.00	11912.0
80.00	8608.0
81.00	10752.0
82.00	2364.0
83.00	2408.0
84.90	1792.0
86.00	4221.0
87.10	1066.0
89.00	402.0
90.90	2281.0
92.10	3269.0
93.00	17880.0
93.80	1444.0
96.10	456.0
98.00	14840.0
99.00	11024.0
99.80	845.0
101.00	5090.0
102.00	490.0
102.90	1547.0
104.00	4022.0
104.90	3207.0
106.10	899.0
107.00	37192.0
108.00	6355.0
109.10	763.0
110.00	54528.0
111.00	10983.0
112.10	959.0
116.00	2201.0
117.00	42520.0
118.10	2701.0
119.80	509.0
122.10	2323.0
123.00	4504.0
124.00	2006.0
125.10	1161.0
126.00	507.0
127.00	104976.0
128.00	7806.0
129.00	44168.0
129.90	3411.0
131.10	676.0
131.90	976.0
133.90	1274.0
135.00	3913.0
135.90	2045.0
137.00	1295.0
139.90	376.0
141.00	7374.0
142.00	1713.0
143.00	1183.0
143.90	613.0
146.00	1014.0
147.00	2311.0
148.00	8335.0
148.90	2276.0
151.10	694.0
152.10	1206.0
152.90	2832.0
153.90	1302.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

155.00	2429.0
156.00	4256.0
157.10	830.0
158.10	1227.0
159.00	505.0
160.00	2525.0
161.10	3168.0
162.00	756.0
163.00	343.0
164.10	410.0
164.90	2346.0
165.90	2091.0
167.00	15447.0
168.00	7002.0
169.10	1699.0
170.80	1189.0
172.00	1039.0
172.90	1147.0
174.10	2431.0
175.00	4100.0
176.00	927.0
176.90	1577.0
177.90	450.0
179.00	10316.0
179.90	6452.0
181.00	2152.0
182.00	575.0
183.10	667.0
184.10	1041.0
185.00	4756.0
186.00	32368.0
187.00	8853.0
188.00	770.0
188.80	1639.0
189.90	654.0
191.00	1198.0
191.90	3528.0
193.00	3649.0
194.00	640.0
196.00	4492.0
196.70	881.0
197.90	181440.0
198.90	14525.0
199.90	1011.0
200.90	584.0
201.70	554.0
203.00	1602.0
204.00	9259.0
205.00	17096.0
206.00	56128.0
207.00	9224.0
208.10	2294.0
208.80	742.0
210.00	885.0
210.60	1504.0
211.10	1939.0
212.00	685.0
213.10	407.0
215.00	940.0
215.80	1238.0
217.00	16287.0
217.90	1859.0
221.10	6847.0
222.00	1916.0
223.00	3309.0
224.00	33544.0
225.00	7777.0
225.90	595.0
227.00	16608.0
228.00	2066.0
229.00	2468.0
229.90	783.0
231.00	1093.0
234.10	866.0
234.90	1106.0
235.90	871.0
236.90	1788.0
238.90	403.0
239.80	364.0
240.80	814.0
242.10	1509.0
243.00	1685.0
244.00	23032.0
245.00	4145.0
246.00	5592.0
246.80	1038.0
248.00	436.0
249.00	560.0
249.90	374.0
254.10	451.0
255.00	124120.0
256.00	17624.0
257.10	1944.0
257.90	7093.0
258.90	1965.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

264.90	3899.0
266.00	557.0
272.00	410.0
272.90	3772.0
274.00	10463.0
275.00	44696.0
276.00	7275.0
277.00	3814.0
278.00	850.0
281.00	657.0
283.10	988.0
283.90	369.0
285.00	1051.0
289.10	320.0
292.80	910.0
294.00	382.0
296.00	17496.0
297.10	2029.0
301.80	552.0
303.10	2140.0
303.90	456.0
313.90	445.0
314.20	436.0
315.00	2132.0
315.80	895.0
316.00	904.0
323.00	5333.0
324.00	1117.0
327.00	1549.0
332.00	645.0
334.00	2789.0
334.90	628.0
341.00	364.0
346.00	1162.0
352.00	975.0
353.00	1021.0
354.10	894.0
365.00	5758.0
366.00	1466.0
372.00	2073.0
373.10	316.0
383.00	363.0
402.00	866.0
403.00	786.0
403.90	732.0
420.90	720.0
421.80	748.0
423.00	4733.0
424.10	1735.0
425.10	330.0
441.00	15719.0
442.10	92232.0
443.10	20520.0
444.00	1779.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

m/z	Abundance
37.00	798.0
38.00	1101.0
39.00	13588.0
40.10	948.0
41.00	567.0
44.10	969.0
45.10	333.0
49.00	1219.0
50.00	41904.0
51.10	165632.0
52.10	8634.0
53.20	361.0
55.10	583.0
56.00	5055.0
57.00	12167.0
58.10	777.0
61.00	2094.0
62.00	1827.0
63.00	5493.0
64.10	1231.0
65.00	3412.0
65.90	310.0
68.00	3092.0
69.00	164352.0
69.90	1016.0
73.10	2084.0
74.00	18192.0
75.00	27288.0
76.00	8558.0
77.00	185408.0
78.00	11275.0
78.90	12987.0
80.00	8225.0
81.00	13280.0
82.10	4317.0
83.00	1659.0
85.10	1965.0
86.00	4580.0
86.90	1772.0
88.10	373.0
90.90	2753.0
91.80	3033.0
93.00	23616.0
94.00	2063.0
95.80	756.0
97.00	421.0
98.00	16118.0
99.00	14354.0
100.00	1356.0
100.90	6663.0
102.90	2259.0
104.00	4225.0
105.10	3621.0
106.10	990.0
107.00	52352.0
108.00	8721.0
108.90	1262.0
110.00	77856.0
110.90	12920.0
112.00	1673.0
112.90	404.0
116.00	2903.0
117.00	57536.0
118.00	4306.0
119.00	607.0
120.00	1063.0
122.00	3889.0
123.00	4461.0
123.90	2085.0
124.90	1469.0
125.80	601.0
127.00	143616.0
128.00	9988.0
129.00	67168.0
130.00	4900.0
130.90	1467.0
131.70	461.0
134.00	1505.0
135.00	4773.0
135.90	1798.0
136.90	3408.0
137.90	510.0
139.90	399.0
141.00	8164.0
142.00	3454.0
143.00	1717.0
143.90	638.0
146.00	1809.0
147.00	4676.0
148.00	13727.0
149.00	2895.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

149.90	440.0
151.20	1386.0
151.90	349.0
152.90	3683.0
153.80	1483.0
155.00	5356.0
156.00	6591.0
157.20	781.0
157.90	1603.0
158.90	774.0
160.10	2901.0
160.90	4321.0
161.90	1511.0
163.80	348.0
164.10	306.0
165.00	3525.0
165.90	2388.0
167.10	19480.0
168.00	10506.0
169.00	1455.0
169.90	682.0
170.80	930.0
171.80	1756.0
172.90	1494.0
173.90	3210.0
175.00	7199.0
175.80	2666.0
176.90	3981.0
177.90	1259.0
179.00	13262.0
180.00	9009.0
180.90	3488.0
181.80	455.0
182.10	439.0
184.00	787.0
185.00	6632.0
186.00	43904.0
187.00	13207.0
187.90	1292.0
189.00	3466.0
190.00	974.0
191.00	1329.0
192.00	4866.0
192.90	4748.0
194.00	1110.0
195.10	1070.0
196.00	8043.0
196.90	2404.0
197.90	288640.0
198.90	20520.0
199.90	1290.0
201.30	819.0
203.00	2607.0
204.00	13328.0
205.00	22072.0
206.00	81776.0
207.00	12757.0
208.00	3619.0
209.00	1159.0
209.90	2165.0
210.80	4808.0
211.70	734.0
214.90	1315.0
216.00	1826.0
217.00	26480.0
218.00	3312.0
219.80	713.0
221.00	12840.0
221.90	2671.0
223.00	6610.0
224.00	50360.0
225.00	14031.0
226.00	2424.0
227.00	26264.0
228.00	2750.0
229.00	4606.0
229.60	382.0
230.10	851.0
230.90	1816.0
231.90	431.0
233.00	677.0
233.90	1886.0
235.00	1937.0
236.00	1705.0
236.90	2508.0
239.10	703.0
239.90	609.0
240.90	1327.0
242.00	2361.0
243.00	3521.0
244.00	35536.0
245.00	4639.0
246.00	8332.0
247.00	1978.0
248.90	1531.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

251.00	383.0
251.70	382.0
253.00	1254.0
254.10	1306.0
255.00	189760.0
256.00	26208.0
257.00	2684.0
258.00	12509.0
259.00	2352.0
259.80	619.0
261.20	338.0
264.90	5239.0
265.90	573.0
271.80	475.0
273.00	6269.0
274.00	14242.0
275.00	73008.0
276.00	10682.0
277.00	7773.0
278.00	1141.0
279.10	491.0
283.00	416.0
283.90	703.0
285.00	1206.0
286.10	327.0
289.10	351.0
289.90	409.0
291.90	342.0
292.90	1801.0
295.00	1204.0
296.00	26600.0
297.00	4212.0
301.00	485.0
301.80	777.0
303.00	2027.0
304.00	668.0
307.90	307.0
309.00	516.0
313.90	1388.0
314.90	2197.0
316.00	1673.0
321.00	750.0
323.00	6267.0
323.90	1158.0
327.00	2338.0
328.00	606.0
331.80	374.0
334.10	5054.0
335.00	1383.0
340.80	839.0
346.00	1630.0
352.00	2024.0
353.00	1329.0
354.10	1428.0
355.00	447.0
365.00	13167.0
365.90	1421.0
370.90	504.0
372.00	3747.0
373.00	1103.0
383.00	1211.0
384.10	363.0
389.70	318.0
390.30	323.0
391.10	345.0
402.00	1181.0
403.00	1749.0
404.10	843.0
421.00	1590.0
422.10	1838.0
423.00	10790.0
424.00	3251.0
425.10	316.0
441.00	30336.0
442.10	189568.0
443.00	34384.0
444.10	3824.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

m/z	Abundance
36.10	373.0
37.10	635.0
38.00	1790.0
39.10	8312.0
40.00	1171.0
41.00	490.0
43.80	644.0
45.00	752.0
49.20	1463.0
50.10	32160.0
51.10	122320.0
52.00	6017.0
55.00	734.0
56.10	3553.0
57.10	8010.0
58.00	382.0
61.00	1120.0
61.90	2178.0
63.00	5491.0
65.00	2031.0
68.00	2117.0
69.00	119152.0
70.00	917.0
73.00	2260.0
74.00	13702.0
75.00	19328.0
76.10	6290.0
77.10	137280.0
78.10	8994.0
79.00	8072.0
80.00	6564.0
81.00	9352.0
82.00	2803.0
83.00	1857.0
84.80	1459.0
86.00	3660.0
86.90	1616.0
87.90	682.0
89.10	370.0
91.00	2199.0
91.90	2415.0
93.00	18288.0
93.90	1058.0
96.10	1121.0
97.20	325.0
98.00	13600.0
99.00	9066.0
99.90	798.0
101.00	4722.0
102.90	1259.0
104.00	3238.0
105.00	4073.0
105.90	1218.0
107.00	39880.0
108.00	5084.0
108.90	822.0
110.00	59600.0
111.00	10206.0
112.00	1089.0
113.10	487.0
116.10	2247.0
117.00	47264.0
118.00	3157.0
120.10	505.0
121.90	2548.0
123.00	3866.0
124.00	2253.0
124.90	1630.0
126.10	923.0
127.00	109336.0
128.00	8527.0
129.00	47320.0
130.00	4575.0
131.00	786.0
132.00	484.0
133.00	493.0
134.00	1079.0
135.00	3382.0
136.10	1895.0
137.00	2305.0
138.00	768.0
138.90	473.0
139.90	938.0
141.00	6880.0
142.00	1747.0
142.80	1923.0
144.00	445.0
145.10	533.0
146.00	1185.0
146.90	3758.0
148.00	11036.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

148.90	2361.0
150.00	560.0
151.10	839.0
152.90	2173.0
154.10	1491.0
155.00	3277.0
156.00	4656.0
156.90	1269.0
157.80	1606.0
159.00	1637.0
159.90	1888.0
160.90	2523.0
162.00	1097.0
165.00	2368.0
165.90	1960.0
167.00	18416.0
168.00	7312.0
169.10	1628.0
170.00	585.0
171.00	366.0
171.80	1432.0
173.10	1880.0
173.80	2137.0
175.00	5388.0
176.10	1627.0
176.90	3106.0
177.90	500.0
178.90	9596.0
180.00	8604.0
181.00	3641.0
182.00	641.0
184.00	919.0
185.00	5063.0
186.00	38608.0
187.00	8700.0
188.20	651.0
189.00	2229.0
189.90	322.0
191.00	1631.0
191.90	4207.0
192.90	3901.0
194.00	905.0
196.10	7433.0
197.00	1683.0
197.90	230784.0
198.90	15763.0
199.90	1558.0
201.50	904.0
202.90	2285.0
204.00	10335.0
205.00	18856.0
206.00	72088.0
207.00	10521.0
208.00	4087.0
209.00	1577.0
209.90	1323.0
210.90	3562.0
211.80	712.0
214.90	1101.0
215.90	1621.0
217.00	23744.0
217.90	3127.0
219.00	438.0
220.00	454.0
221.00	7821.0
221.90	2542.0
223.00	5443.0
224.00	42848.0
225.10	9108.0
226.00	1509.0
227.00	21328.0
228.10	2930.0
228.90	4777.0
230.00	1118.0
231.00	1612.0
234.00	1560.0
235.00	913.0
235.90	845.0
237.00	2009.0
238.90	860.0
239.90	1015.0
240.90	1100.0
241.90	1390.0
242.90	3142.0
244.00	33304.0
245.00	4570.0
245.90	7618.0
246.80	1122.0
247.80	479.0
249.00	1190.0
250.90	315.0
251.90	301.0
252.80	728.0
254.10	1470.0
255.00	168448.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

256.00	23440.0
257.00	2204.0
258.00	10105.0
258.90	2111.0
260.00	614.0
264.90	3856.0
266.90	388.0
271.10	414.0
272.00	723.0
273.00	4807.0
274.00	12467.0
275.00	68264.0
276.00	9092.0
277.00	7034.0
278.00	1110.0
279.10	333.0
281.00	747.0
283.00	1055.0
284.00	417.0
284.90	852.0
289.90	477.0
291.80	379.0
293.00	1804.0
293.80	310.0
294.90	411.0
296.00	23760.0
297.00	3777.0
298.00	335.0
303.00	1763.0
304.00	366.0
308.00	503.0
310.00	331.0
312.90	457.0
313.90	1857.0
315.00	3122.0
315.90	1308.0
321.00	313.0
321.80	337.0
323.00	7738.0
324.10	1444.0
327.10	1835.0
327.90	949.0
332.00	389.0
333.10	631.0
333.90	5289.0
335.00	1406.0
338.90	319.0
341.00	604.0
341.90	380.0
345.80	1634.0
346.90	600.0
352.00	2397.0
353.10	811.0
354.10	1626.0
365.00	9287.0
365.90	1768.0
369.80	313.0
371.20	328.0
372.10	3971.0
373.00	944.0
382.90	1002.0
383.90	342.0
390.10	548.0
392.00	606.0
400.90	388.0
402.00	1084.0
403.10	1661.0
404.00	748.0
420.90	1072.0
422.00	1841.0
423.10	11181.0
424.10	3117.0
441.00	31984.0
442.10	198080.0
443.00	34432.0
444.00	3820.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07

m/z	Abundance
40.00	761.0
41.00	346.0
44.10	443.0
73.00	519.0
193.00	322.0
207.10	1164.0

Instrument :
BNA_M
ClientSampleId :
DFTPP07