

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
 Data File : BM029670.D
 Acq On : 27 Apr 2021 12:45
 Operator : CG/JU
 Sample : PB136001BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB136001BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.210	389	395	411	rBV	1052083	1511960	34.75%	8.758%
2	6.793	657	664	684	rBV	950362	1546610	35.54%	8.959%
3	7.610	797	803	818	rVB	206196	337587	7.76%	1.956%
4	8.769	991	1000	1012	rBV	564034	982594	22.58%	5.692%
5	10.392	1269	1276	1294	rBV	256197	442212	10.16%	2.562%
6	12.875	1692	1698	1716	rBV	1785227	2734664	62.84%	15.841%
7	14.263	1927	1934	1948	rBV	435724	650143	14.94%	3.766%
8	15.751	2181	2187	2210	rBV	1420078	2113315	48.56%	12.242%
9	17.004	2394	2400	2414	rBV	527404	774643	17.80%	4.487%
10	19.639	2843	2848	2859	rBV	3536246	4351555	100.00%	25.208%
11	21.192	3107	3112	3120	rBV	687092	914616	21.02%	5.298%
12	23.374	3477	3483	3491	rBV2	490778	902992	20.75%	5.231%




Sum of corrected areas: 17262891

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
Data File : BM029670.D
Acq On : 27 Apr 2021 12:45
Operator : CG/JU
Sample : PB136001BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136001BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

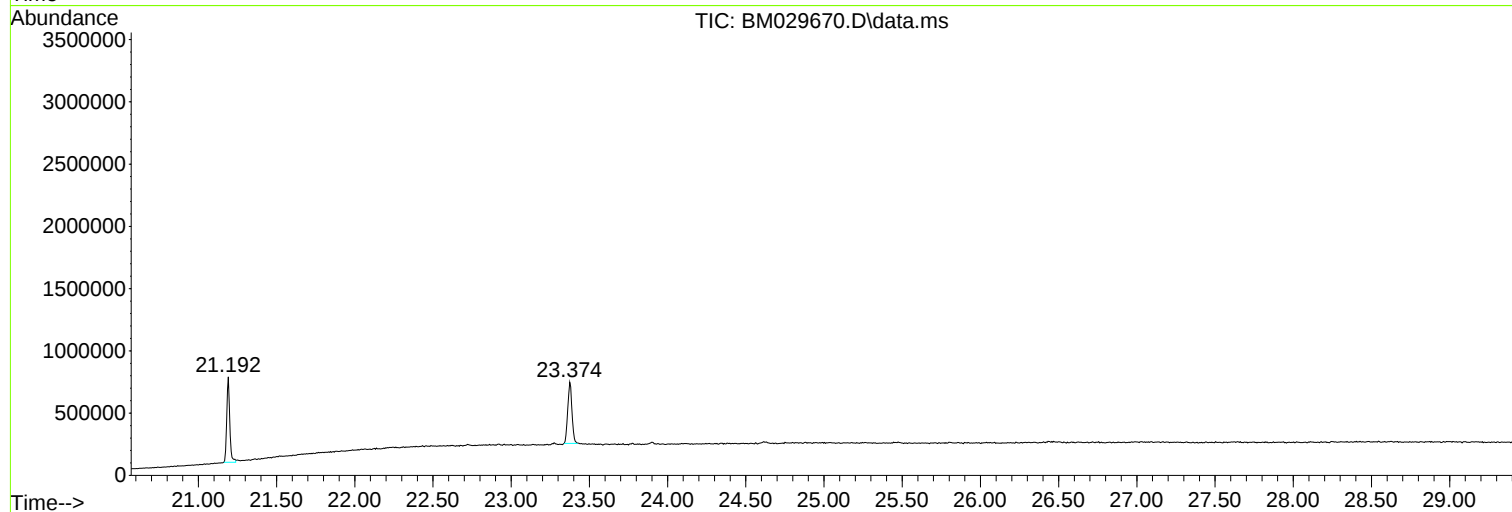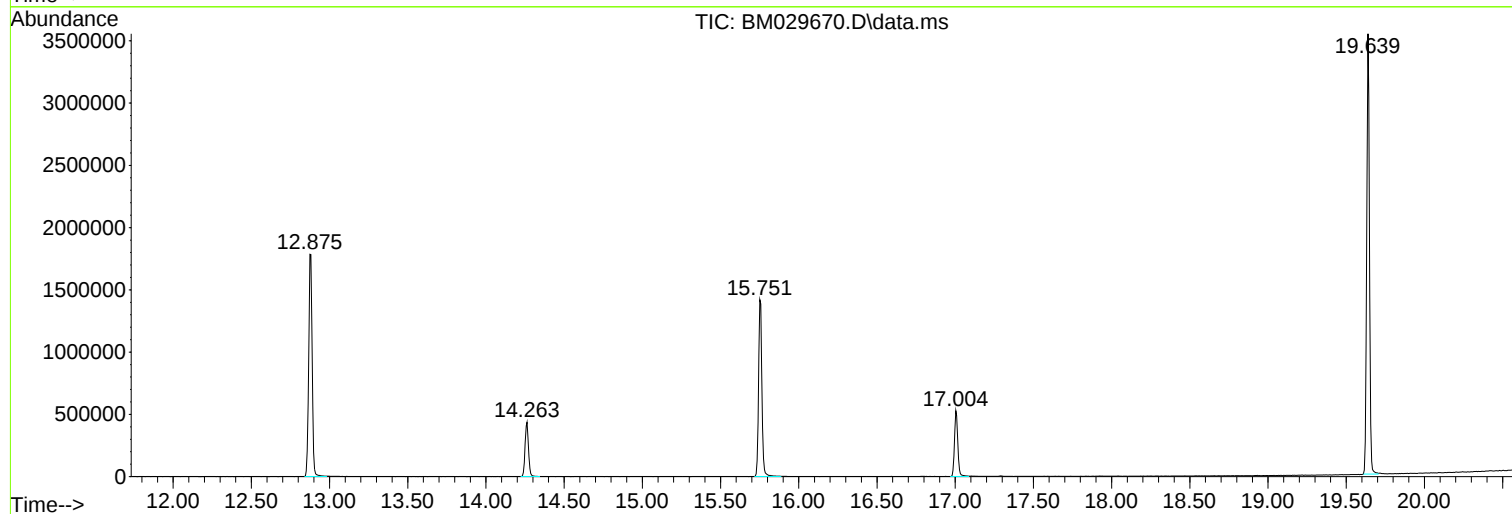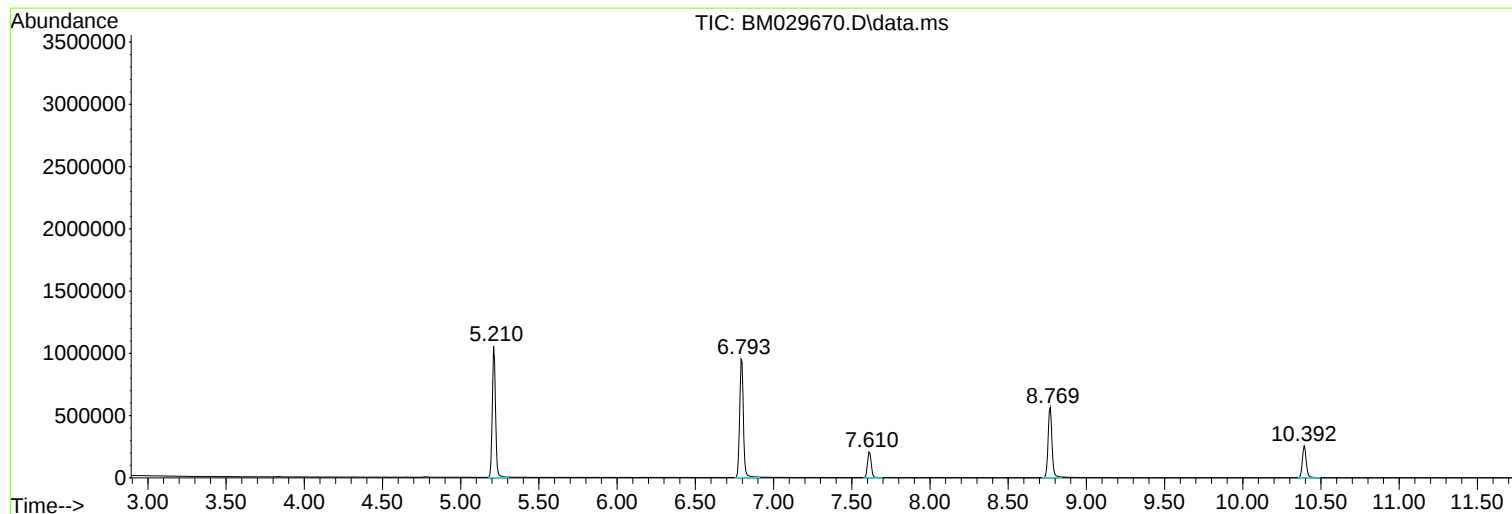

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
Data File : BM029670.D
Acq On : 27 Apr 2021 12:45
Operator : CG/JU
Sample : PB136001BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136001BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
Data File : BM029670.D
Acq On : 27 Apr 2021 12:45
Operator : CG/JU
Sample : PB136001BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136001BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------