

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
 Data File : BM029672.D
 Acq On : 27 Apr 2021 14:03
 Operator : CG/JU
 Sample : PB136013BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB136013BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.210	389	395	408	rBV	1216856	1720177	38.38%	9.388%
2	6.793	657	664	682	rBV	1090974	1732095	38.64%	9.453%
3	7.610	797	803	818	rVB	223466	362987	8.10%	1.981%
4	8.769	992	1000	1014	rBV	659592	1117487	24.93%	6.099%
5	10.392	1267	1276	1293	rBV	272837	468645	10.46%	2.558%
6	12.875	1691	1698	1717	rBV	2022406	3035531	67.72%	16.567%
7	14.257	1927	1933	1948	rBV	428028	667204	14.89%	3.641%
8	15.751	2181	2187	2210	rBV	1632131	2284688	50.97%	12.469%
9	17.004	2394	2400	2414	rBV	498756	751334	16.76%	4.101%
10	19.639	2842	2848	2868	rBV	3761327	4482246	100.00%	24.463%
11	21.192	3107	3112	3119	rBV	624907	850048	18.96%	4.639%
12	23.374	3477	3483	3494	rVB	449531	850035	18.96%	4.639%




Sum of corrected areas: 18322477

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
Data File : BM029672.D
Acq On : 27 Apr 2021 14:03
Operator : CG/JU
Sample : PB136013BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136013BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

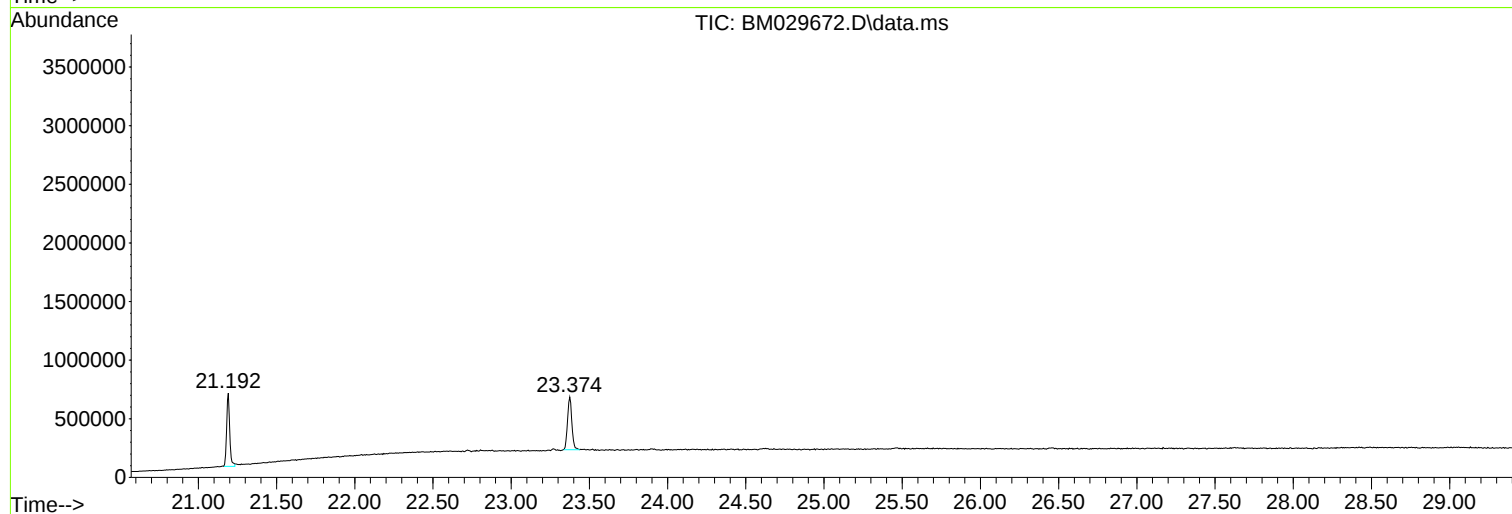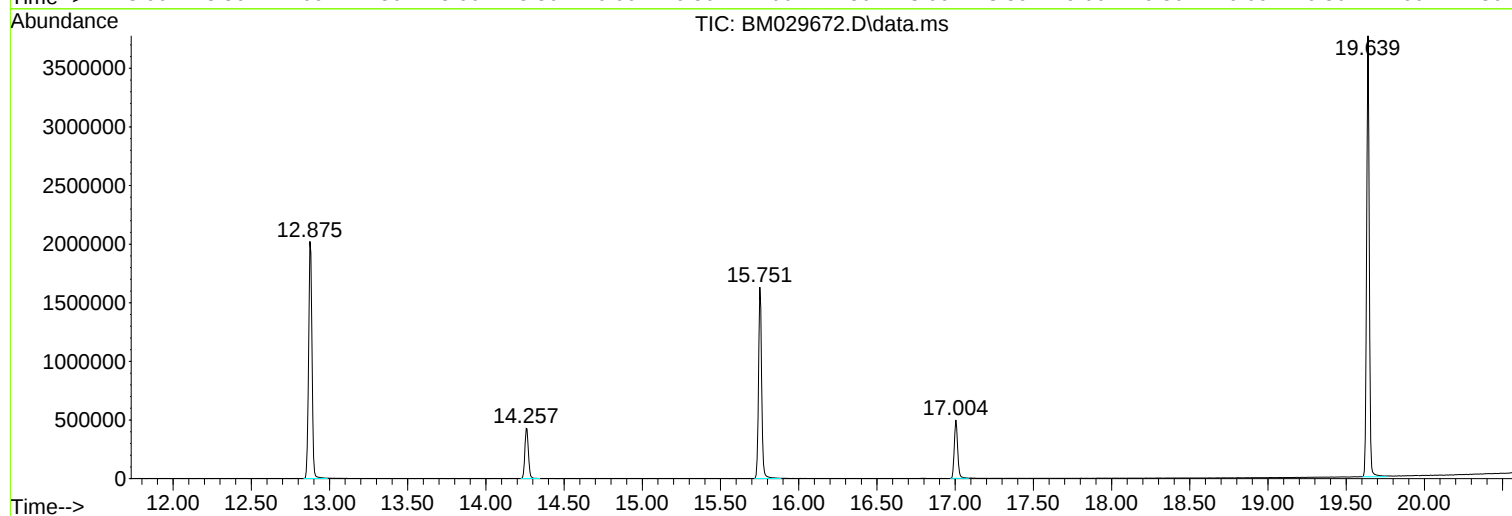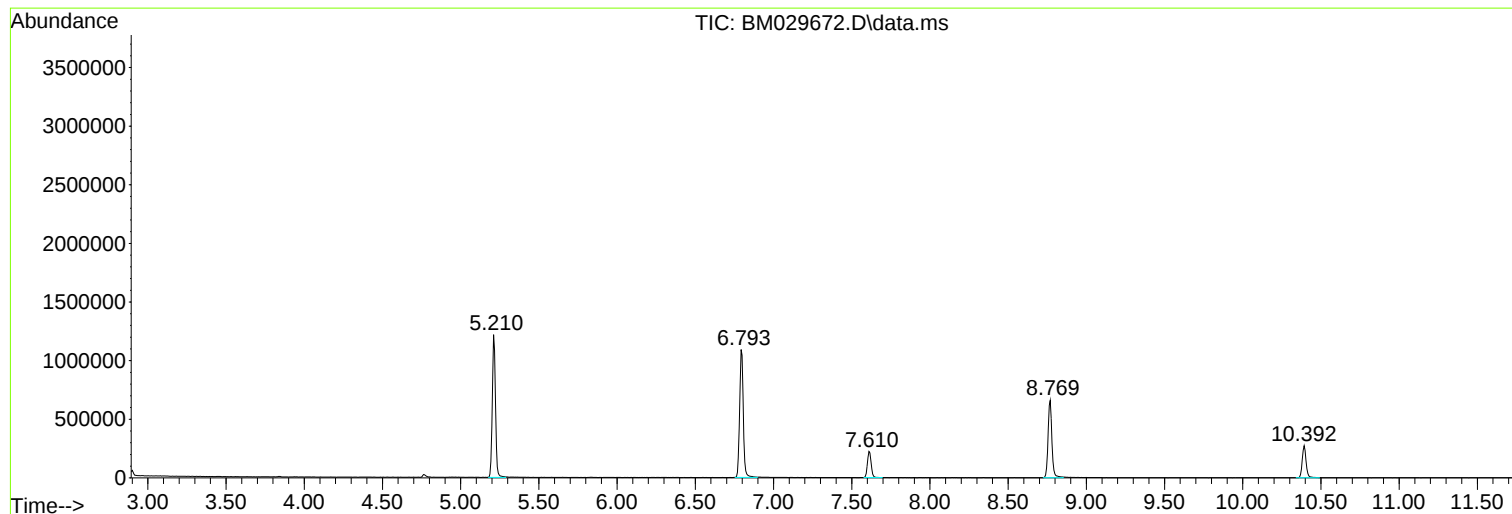

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
Data File : BM029672.D
Acq On : 27 Apr 2021 14:03
Operator : CG/JU
Sample : PB136013BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136013BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
Data File : BM029672.D
Acq On : 27 Apr 2021 14:03
Operator : CG/JU
Sample : PB136013BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB136013BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------