


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
 Data File : BM029668.D
 Acq On : 27 Apr 2021 10:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 26 15:01:01 2021

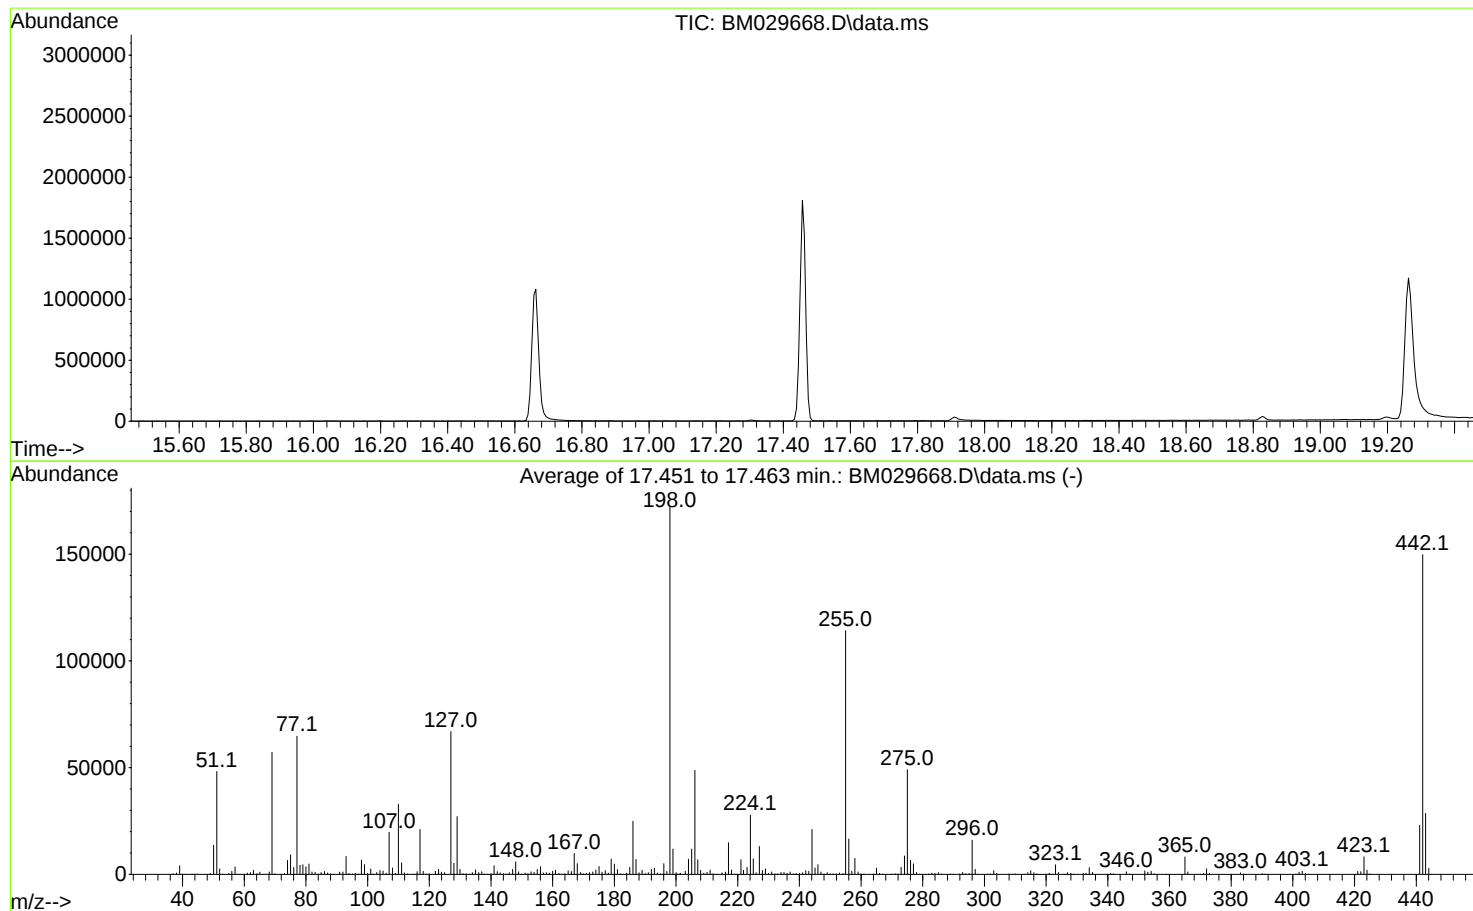

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.0	48195	PASS
68	69	0.00	2	2.0	1126	PASS
69	198	0.00	100	33.2	57189	PASS
70	69	0.00	2	0.6	318	PASS
127	198	10	80	38.8	66832	PASS
197	198	0.00	2	0.8	1376	PASS
198	198	100	100	100.0	172331	PASS
199	198	5	9	6.9	11818	PASS
275	198	10	60	28.5	49037	PASS
365	198	1	100	4.8	8209	PASS
441	198	0.01	100	13.4	23015	PASS
442	442	50	100	100.0	149771	PASS
443	442	15	24	19.1	28579	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/27/2021	BNA_M	<u>BM029668.D</u>
Compound Name	Response	Retention Time
DDT	699318	20.49
DDD	4250	20.05
DDE	804	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5054	704372	0.72

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
Data File : BM029668.D
Acq On : 27 Apr 2021 10:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 27 11:40:53 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 26 15:01:01 2021
Response via : Initial Calibration

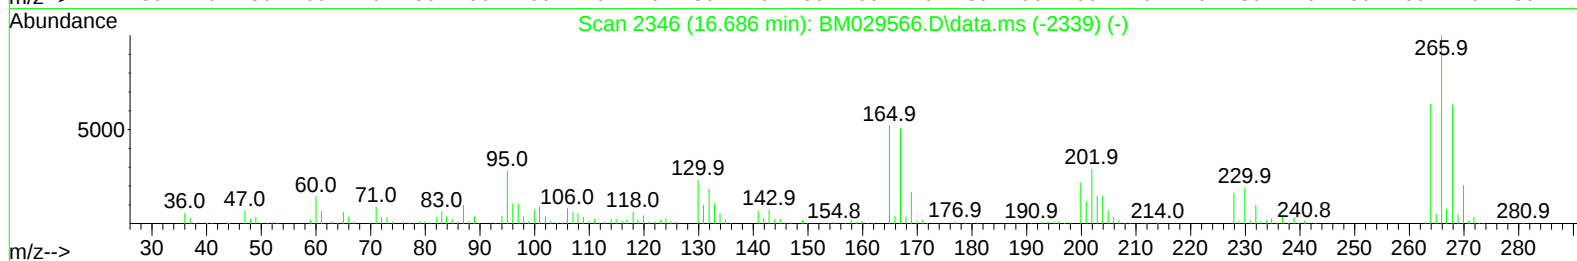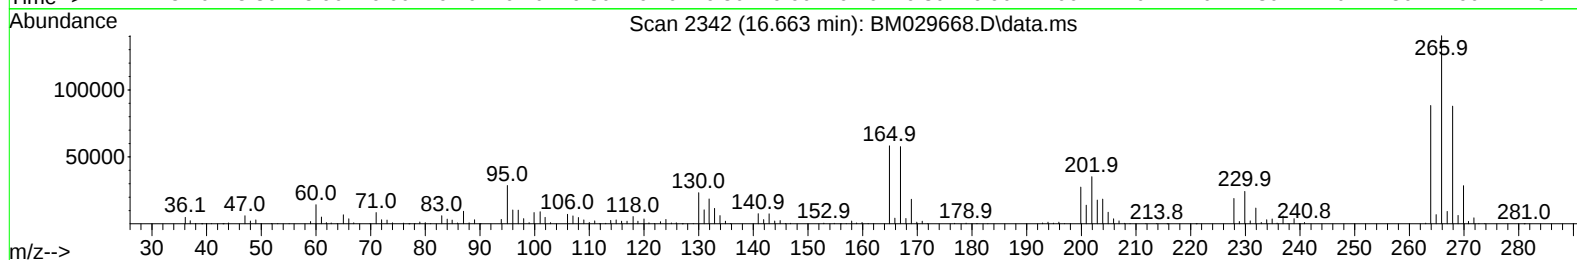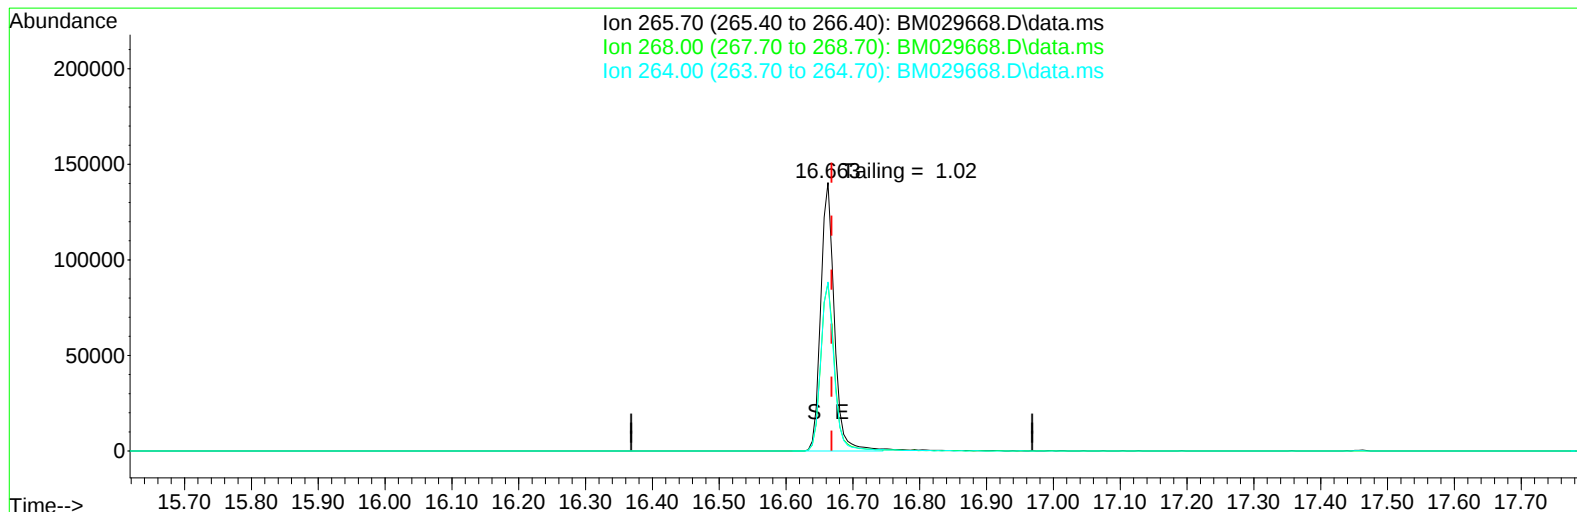

TIC: BM029668.D\data.ms

(70) Pentachlorophenol (C)

16.663min (-0.006) 141783.88 ng




response 200568

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	62.60
264.00	64.90	62.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042721\
 Data File : BM029668.D
 Acq On : 27 Apr 2021 10:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 27 11:40:53 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 26 15:01:01 2021
 Response via : Initial Calibration

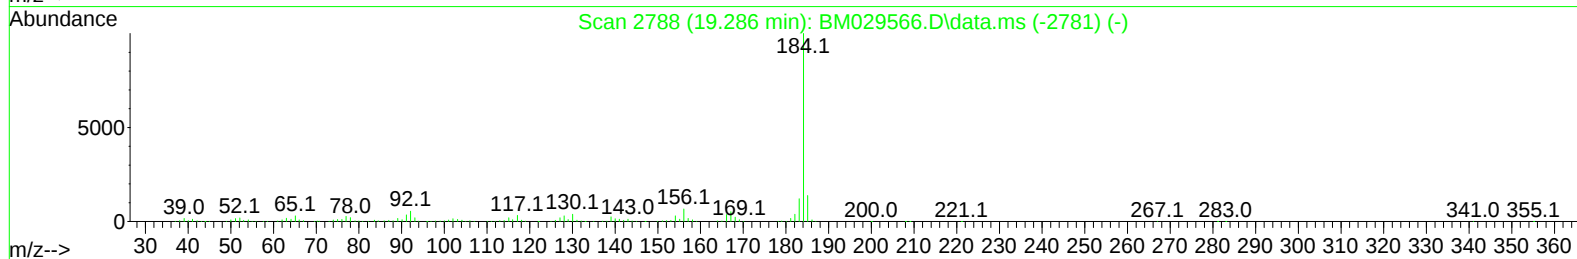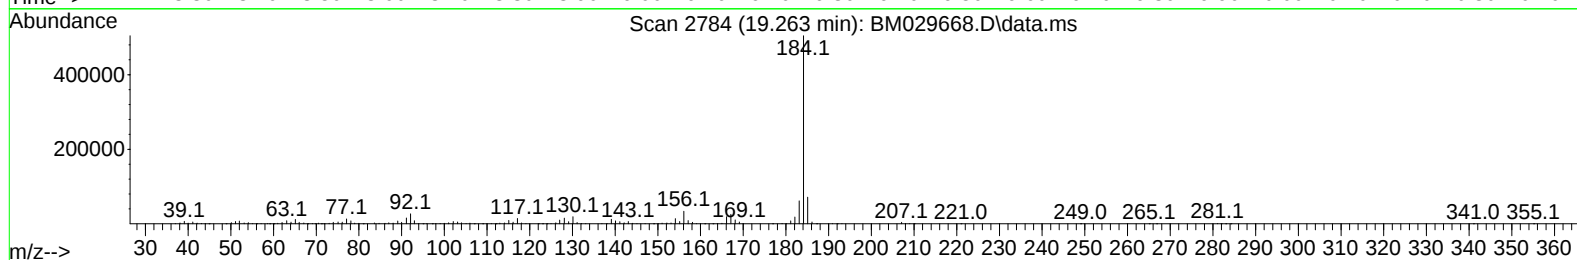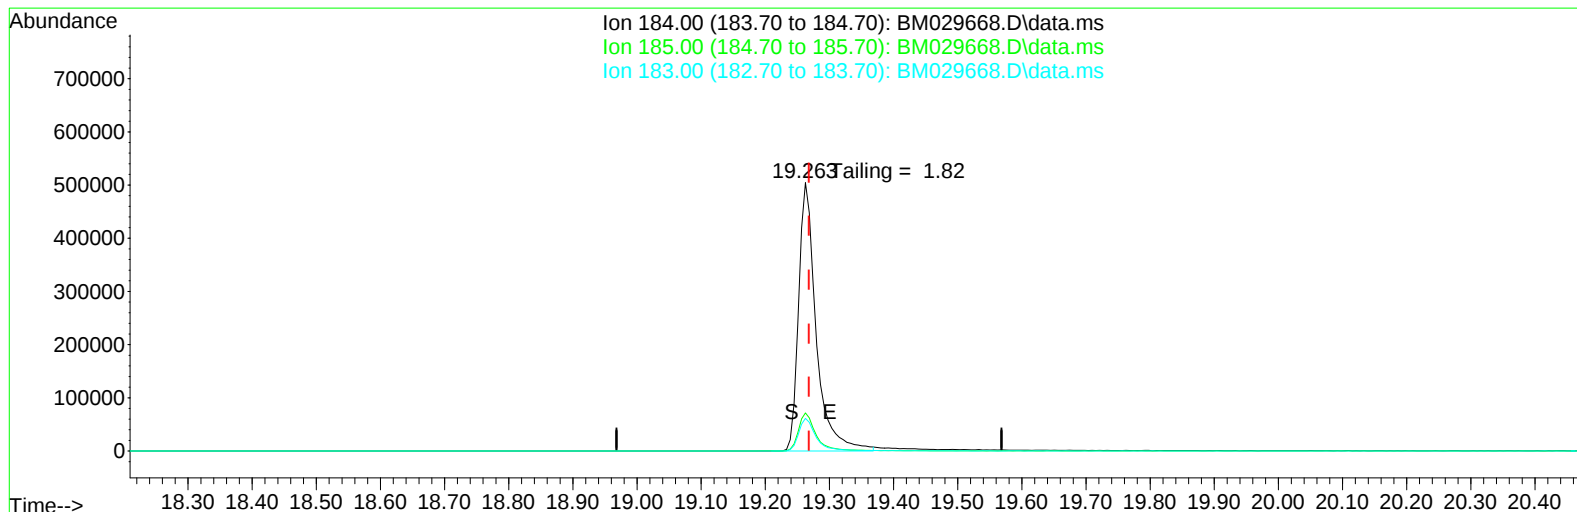

TIC: BM029668.D\data.ms

(77) Benzidine

19.263min (-0.006) 165166.07 ng

response 986140

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	14.19
183.00	12.30	12.21
0.00	0.00	0.00