
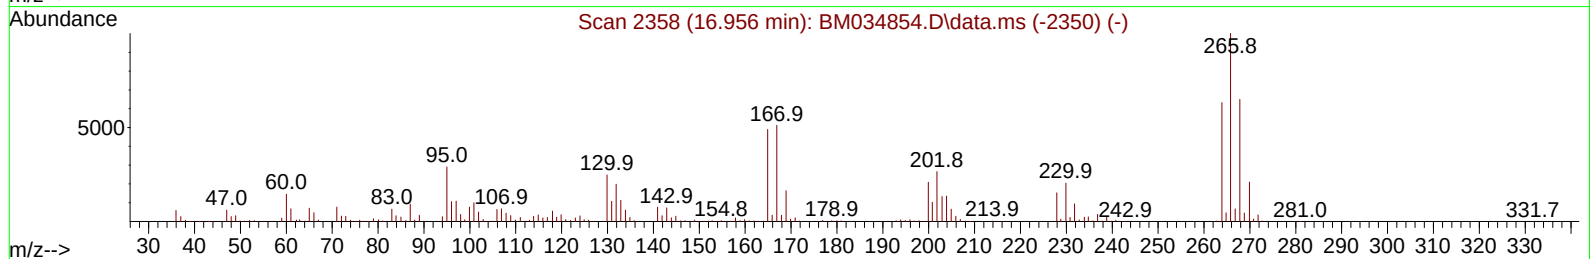
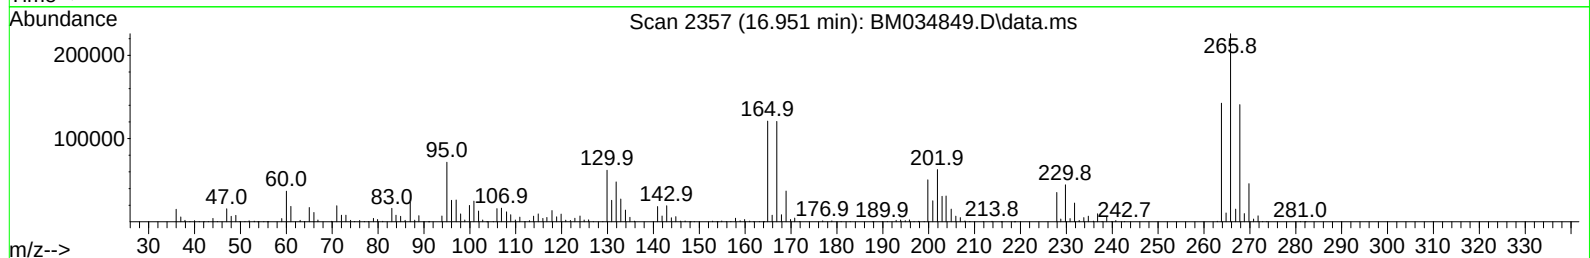


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042722\
Data File : BM034849.D
Acq On : 27 Apr 2022 12:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 08:35:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration

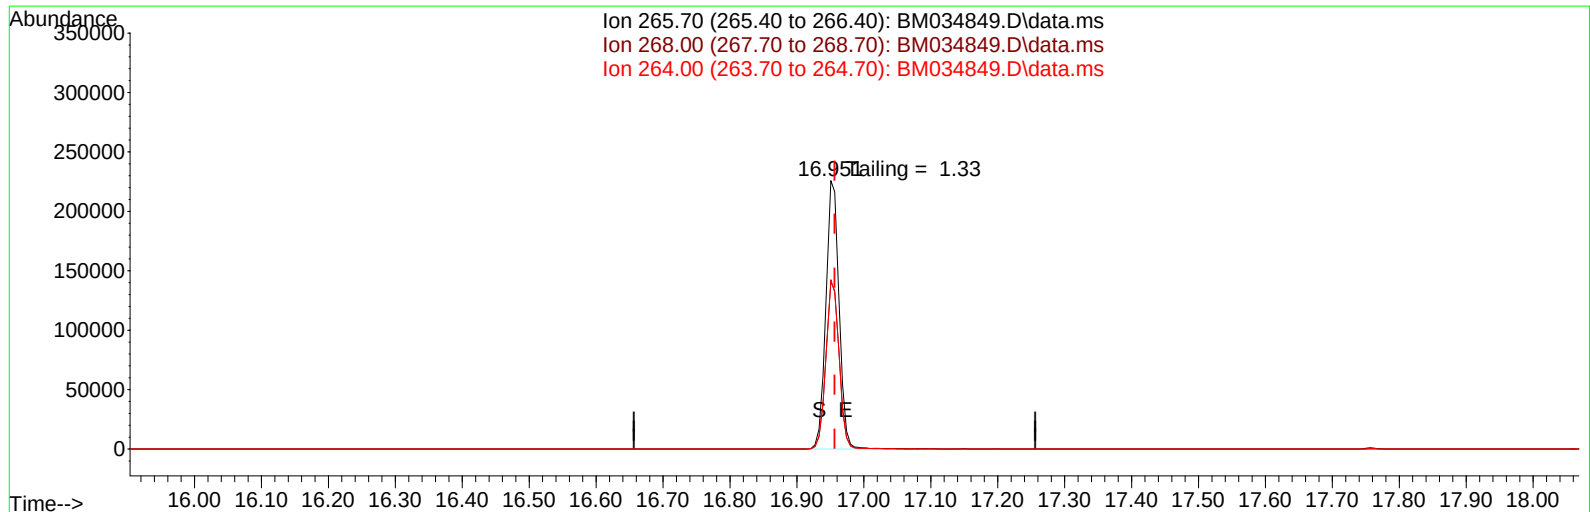

TIC: BM034849.D\data.ms

(70) Pentachlorophenol (C)




16.951min (-0.006) 0.00 ng

response 311009

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.31
264.00	63.30	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042722\
Data File : BM034849.D
Acq On : 27 Apr 2022 12:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 28 08:35:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration

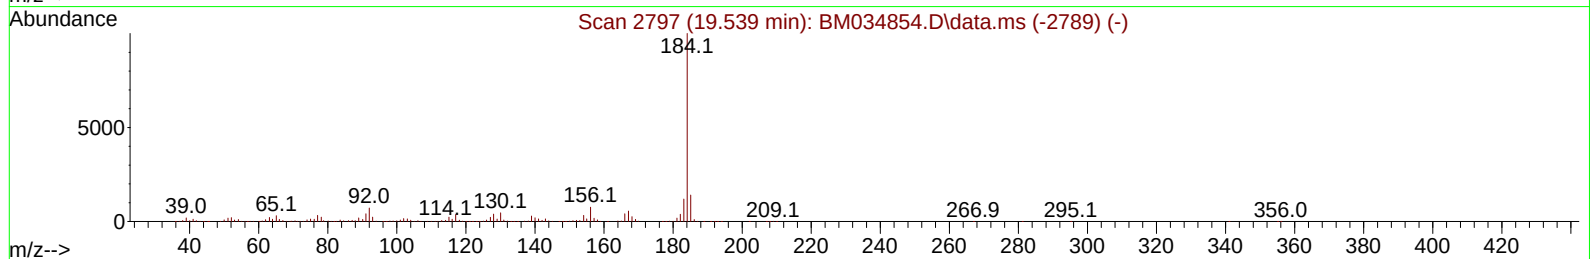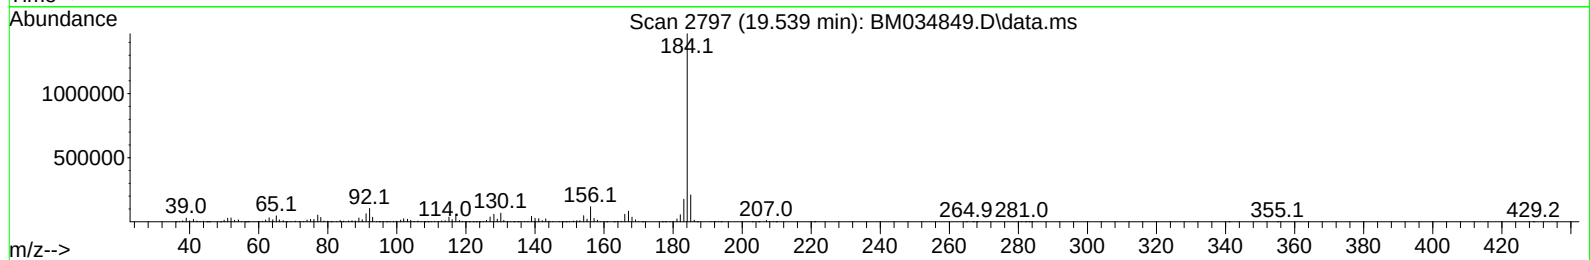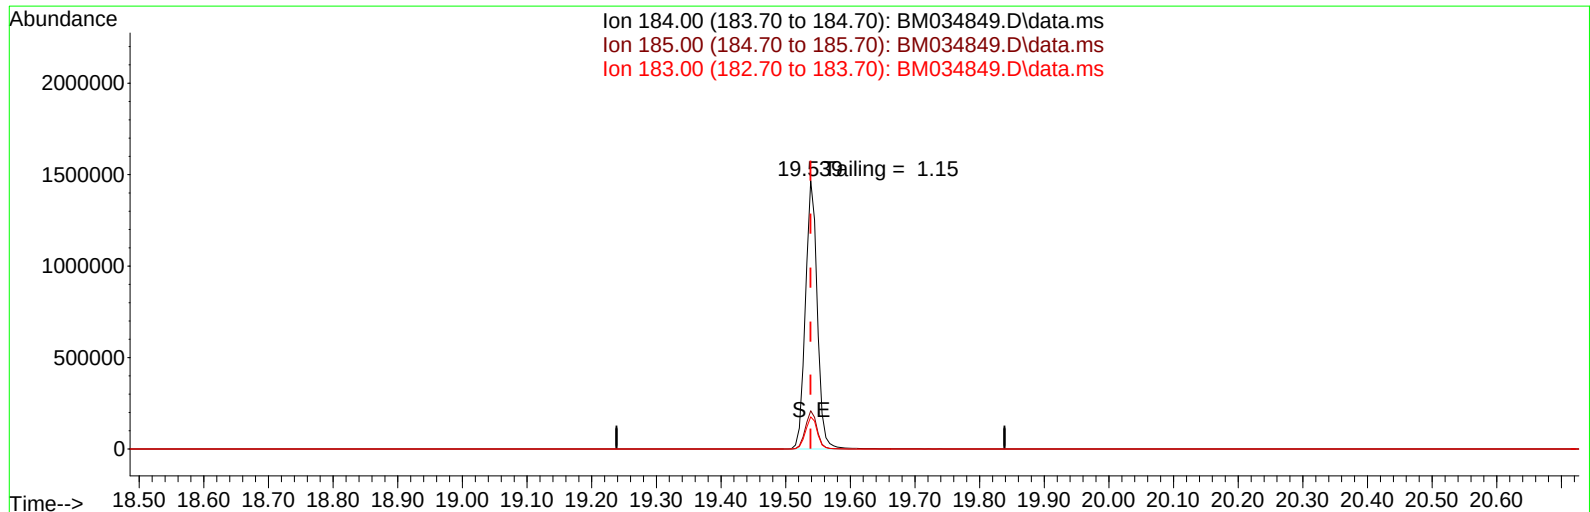

TIC: BM034849.D\data.ms

(77) Benzidine**19.539min (+ 0.000) 945811.57 ng****response 1878105**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.28
183.00	11.90	12.00
0.00	0.00	0.00