
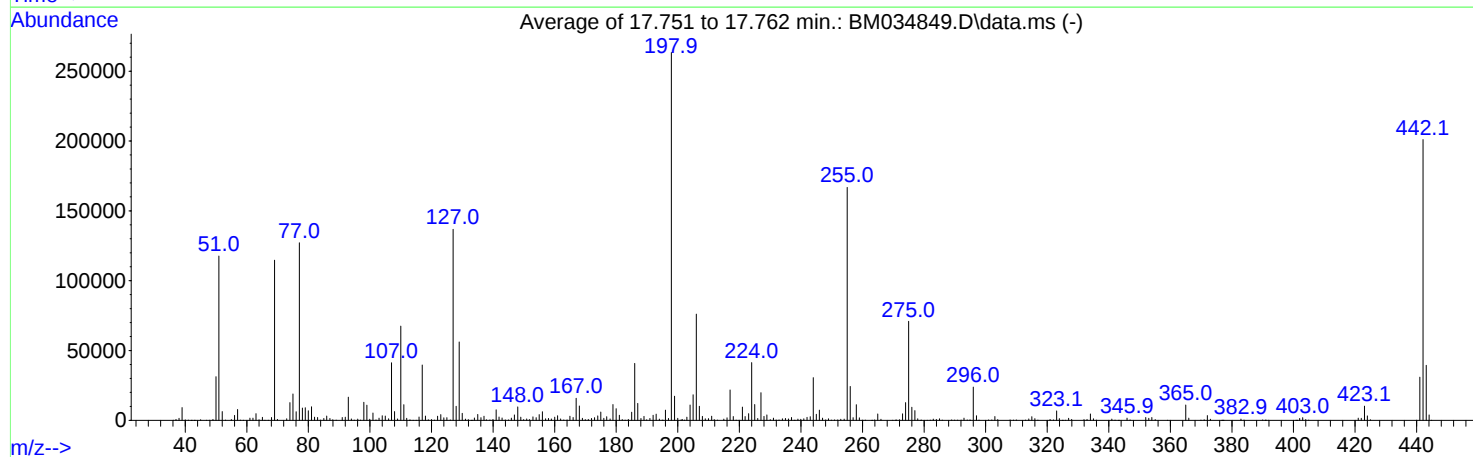


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042722\
 Data File : BM034849.D
 Acq On : 27 Apr 2022 12:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 28 01:51:59 2022

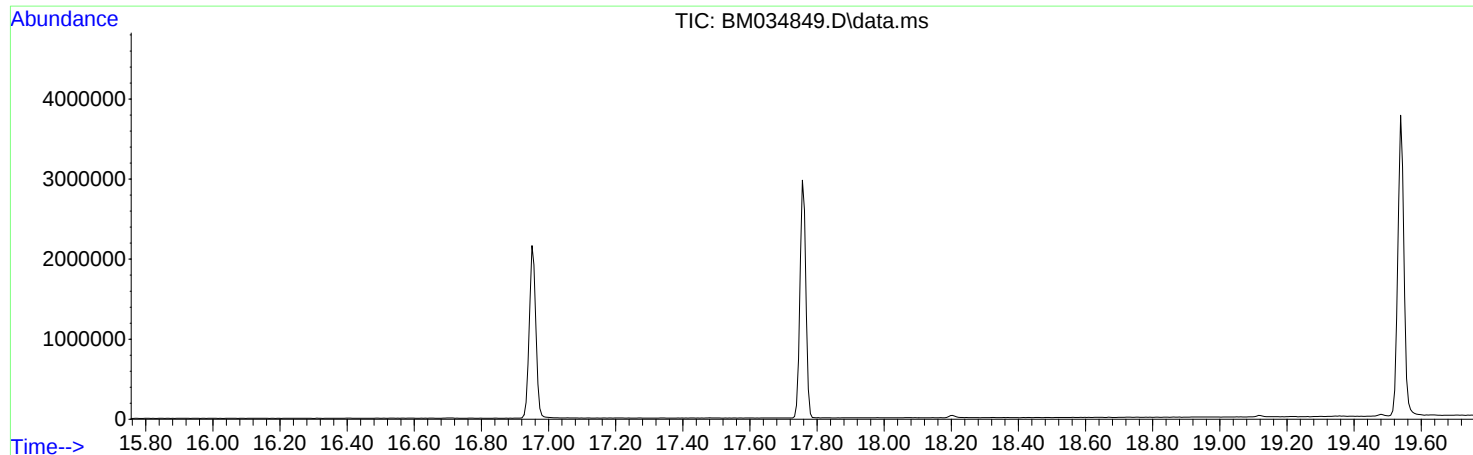




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2487

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	117701	PASS
68	69	0.00	2	1.8	2021	PASS
69	198	0.00	100	43.5	114661	PASS
70	69	0.00	2	0.6	647	PASS
127	198	10	80	51.9	136819	PASS
197	198	0.00	2	0.5	1390	PASS
198	198	100	100	100.0	263381	PASS
199	198	5	9	6.6	17308	PASS
275	198	10	60	26.9	70904	PASS
365	198	1	100	4.2	11002	PASS
441	198	0.01	100	11.8	30987	PASS
442	442	50	100	100.0	201037	PASS
443	442	15	24	19.6	39451	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042722\
 Data File : BM034849.D
 Acq On : 27 Apr 2022 12:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 28 08:35:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 28 01:51:59 2022
 Response via : Initial Calibration

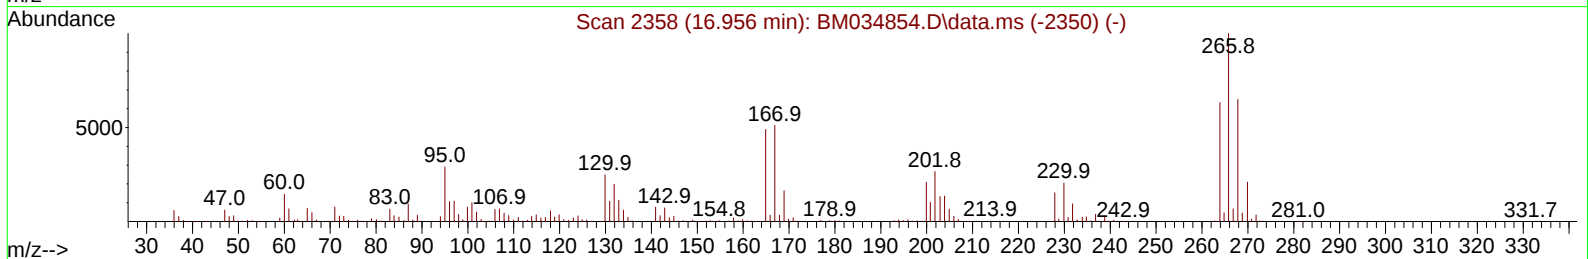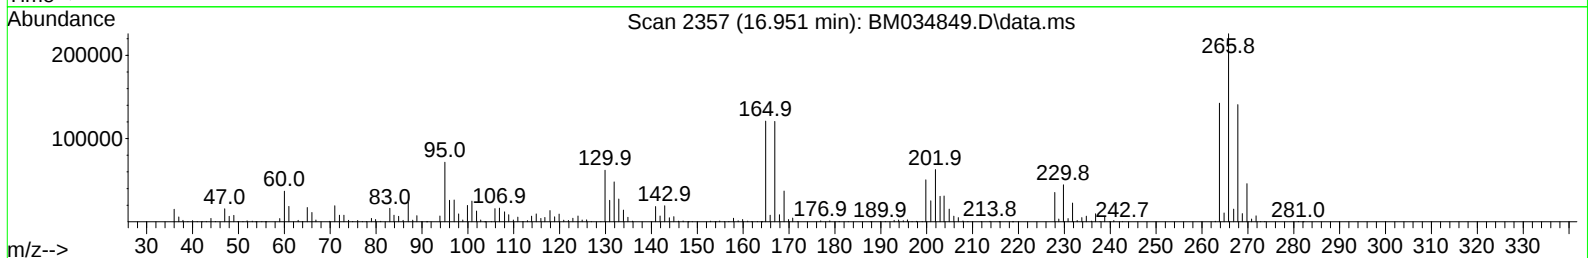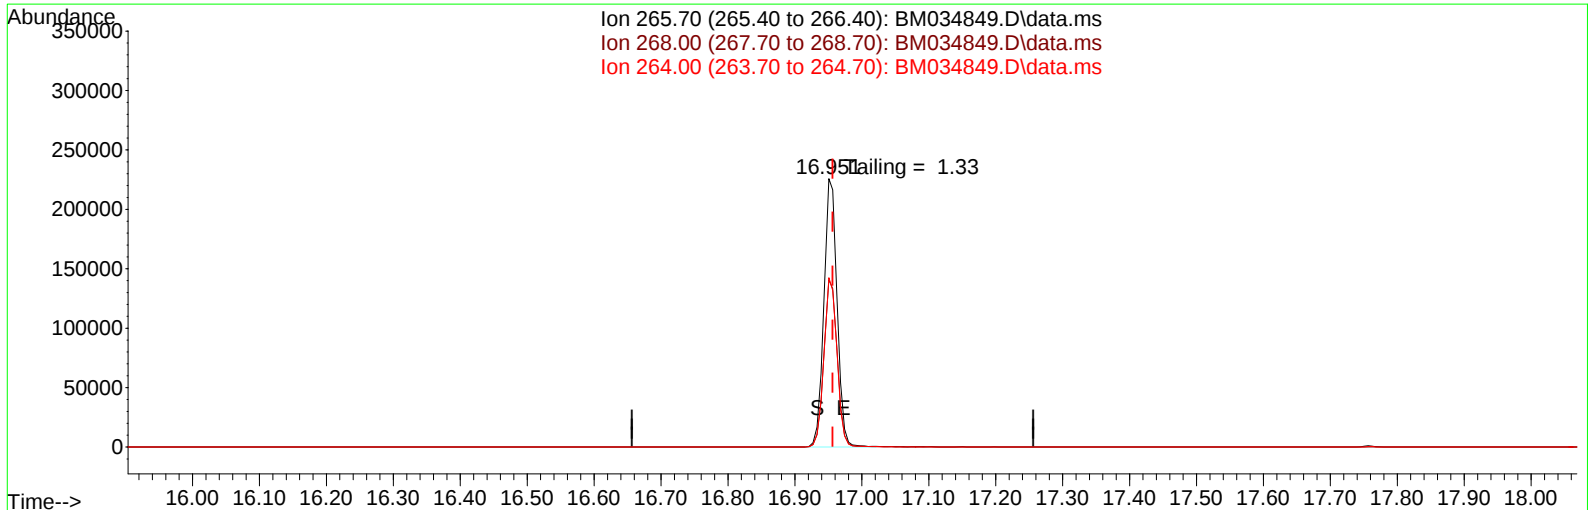

TIC: BM034849.D\data.ms

(70) Pentachlorophenol (C)

16.951min (-0.006) 0.00 ng




response 311009

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.31
264.00	63.30	63.08
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042722\
Data File : BM034849.D
Acq On : 27 Apr 2022 12:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 28 08:35:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration

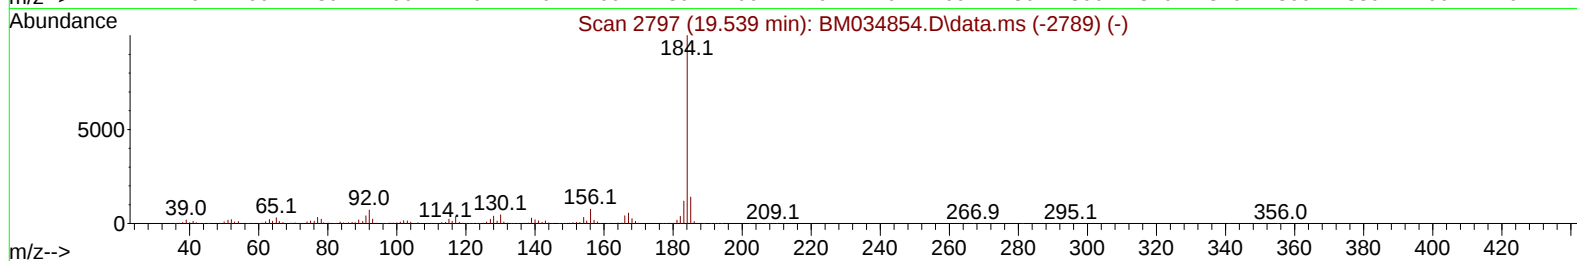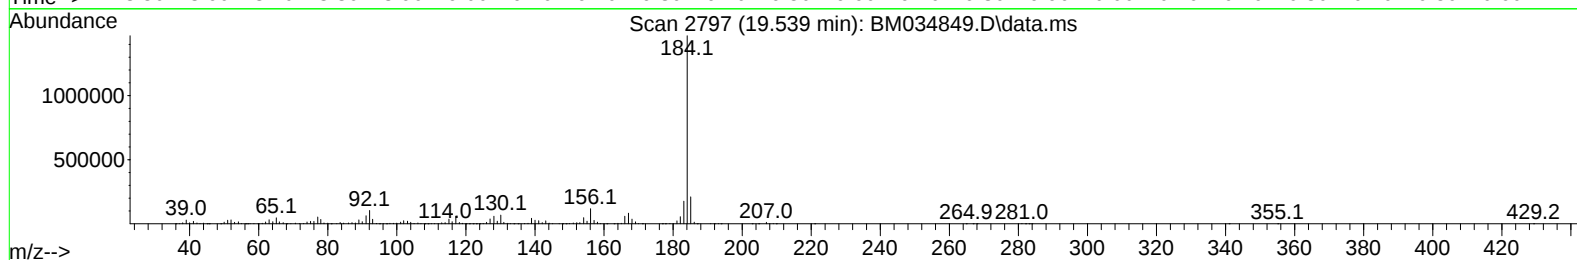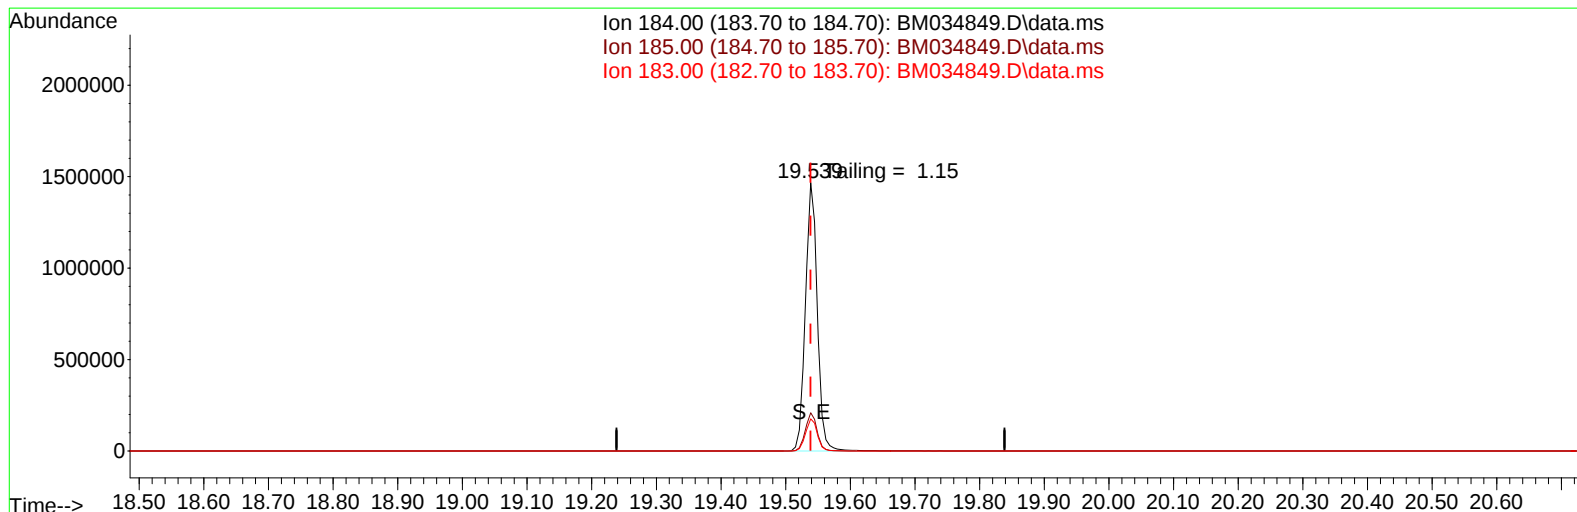

TIC: BM034849.D\data.ms

(77) Benzidine

19.539min (+ 0.000) 945811.57 ng

response 1878105

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.28
183.00	11.90	12.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/27/2022	BNA_M	<u>BM034849.D</u>
Compound Name	Response	Retention Time
DDT	929879	20.78
DDD	4254	20.392
DDE	0	19.853
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4254	934133	0.46

Instrument :
BNA_M
ClientSampleId :
DFTPP