

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042723\
 Data File : BM039710.D
 Acq On : 27 Apr 2023 17:48
 Operator : CG/JU
 Sample : PB152345BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK345

Quant Time: Apr 28 02:34:11 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 28 02:30:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	3763	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.601	136	13790	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.455	164	7745	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.204	188	16595	0.400	ng/ul	-0.01
17) Chrysene-d12	21.423	240	11586	0.400	ng/ul	0.01
23) Perylene-d12	23.758	264	12495	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.189	96	26745	4.823	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.250	152	4583	0.259	ng/ul	0.03
18) Fluoranthene-d10	19.243	212	10538	0.338	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.601	202	1698	0.038	ng/ul#	1
26) Benzo(a)pyrene	23.592	252	3151	0.080	ng/ul#	52


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042723\
Data File : BM039710.D
Acq On : 27 Apr 2023 17:48
Operator : CG/JU
Sample : PB152345BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK345

Quant Time: Apr 28 02:34:11 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:30:02 2023
Response via : Initial Calibration

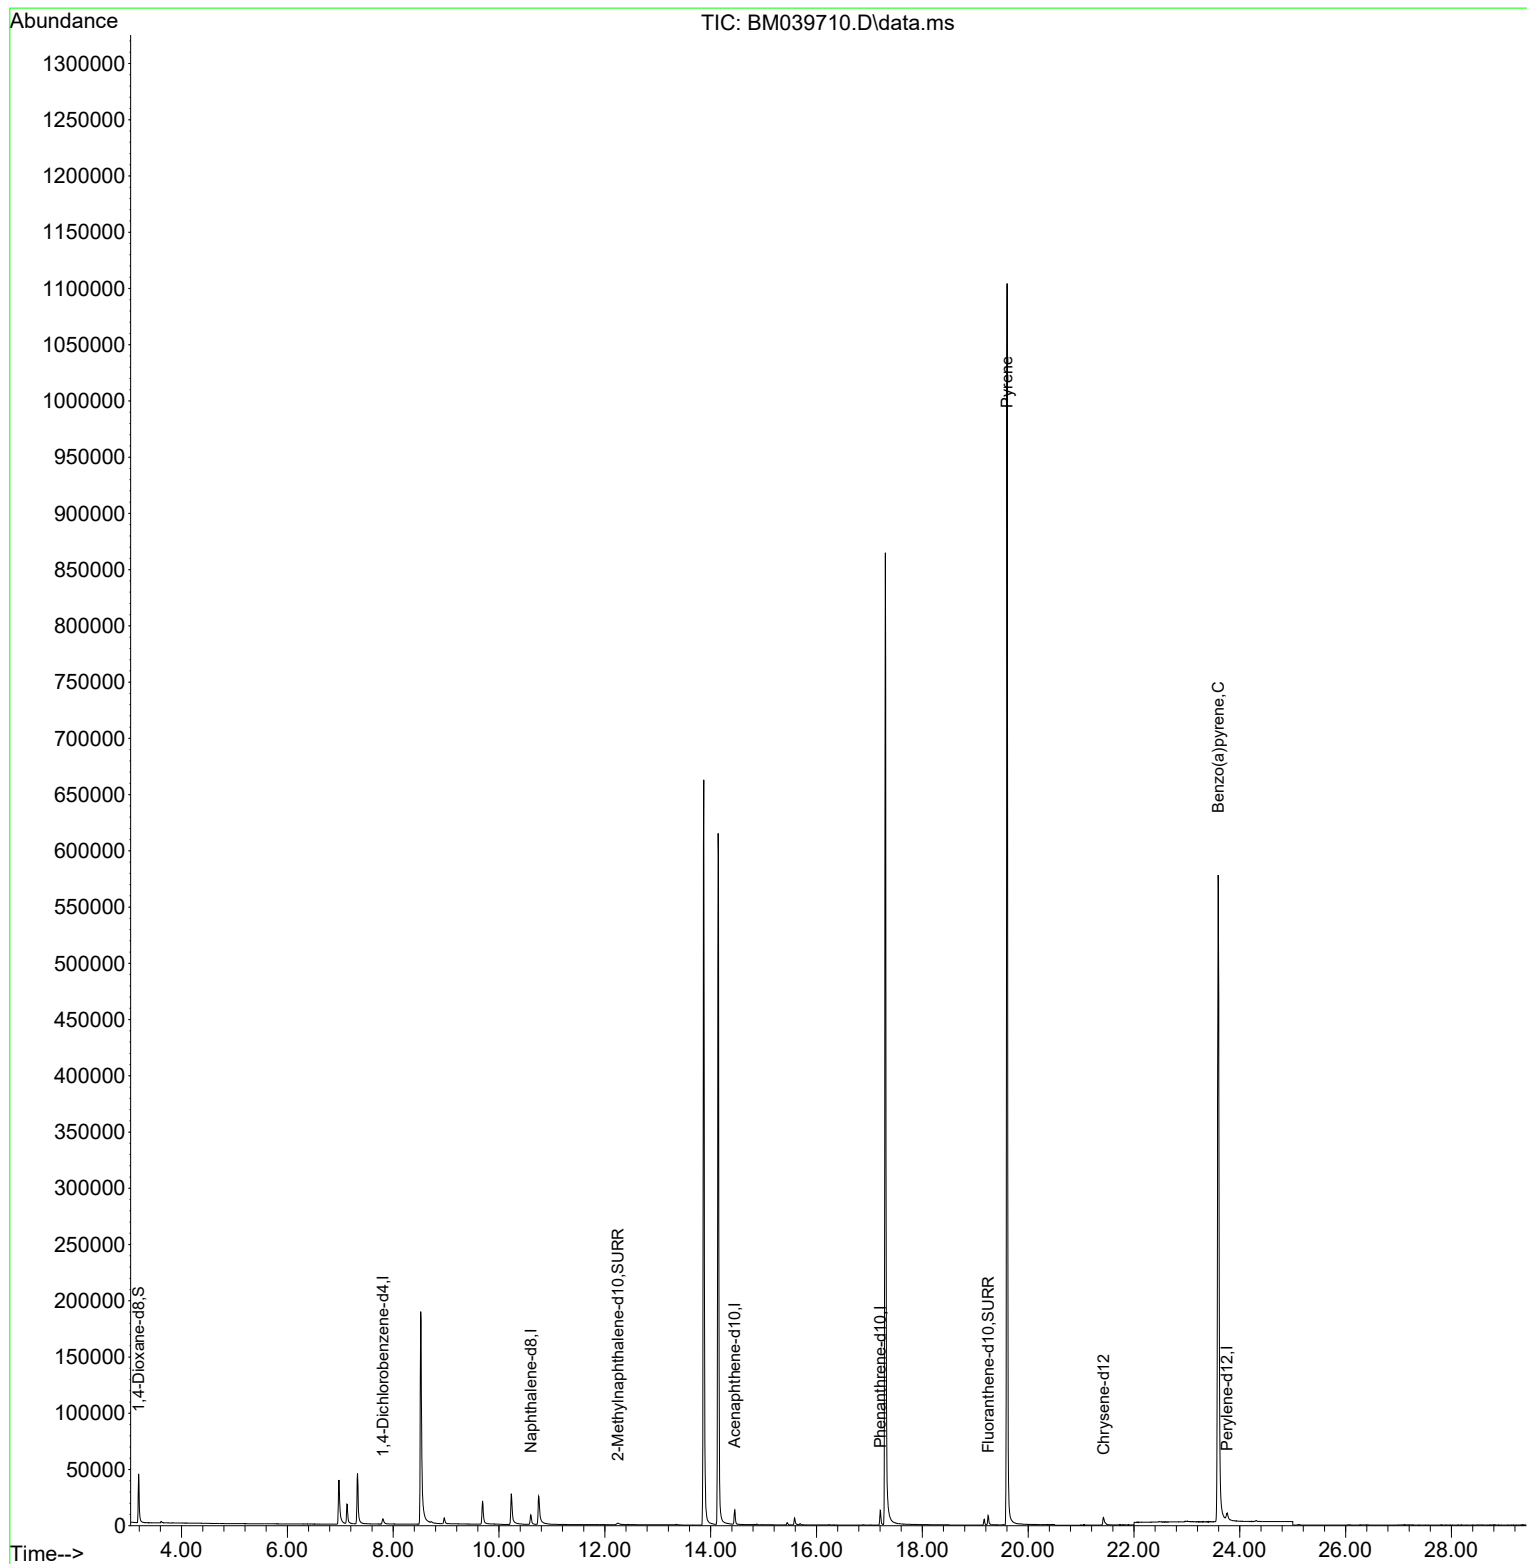

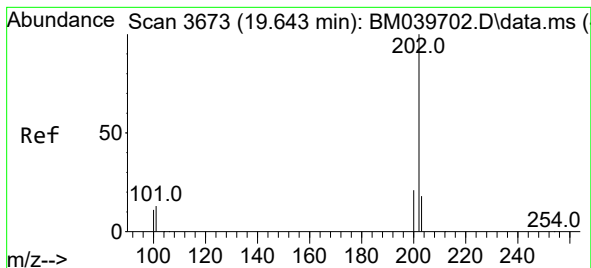

#20

Pyrene

Concen: 0.038 ng/ul

RT: 19.601 min Scan# 3

Delta R.T. -0.042 min

Lab File: BM039710.D

Acq: 27 Apr 2023 17:48

Instrument :

BNA_M

ClientSampleId :

SBLK345





Tgt Ion:202 Resp: 1698

Ion Ratio Lower Upper

202 100

101 168.2 10.9 16.3#

100 1253.0 8.9 13.3#

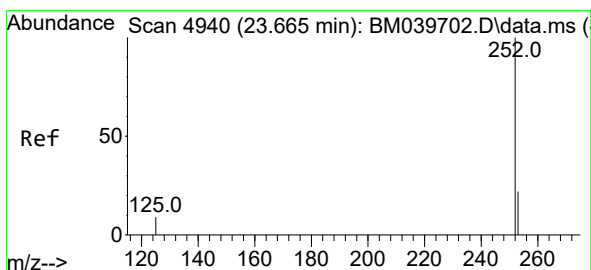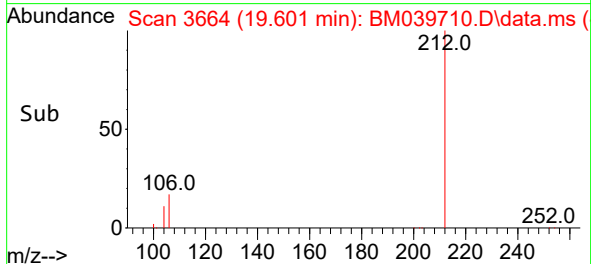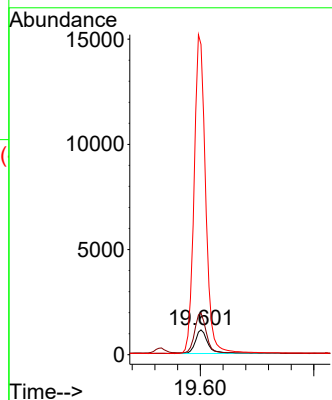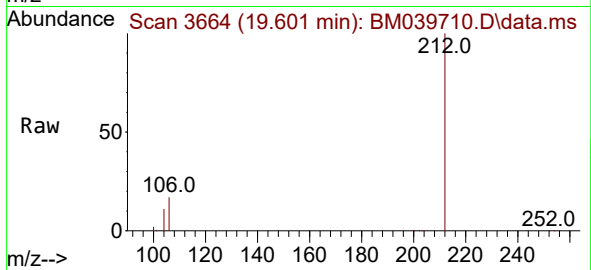

#26

Benzo(a)pyrene

Concen: 0.080 ng/ul

RT: 23.592 min Scan# 4915

Delta R.T. -0.073 min

Lab File: BM039710.D

Acq: 27 Apr 2023 17:48

Tgt Ion:252 Resp: 3151

Ion Ratio Lower Upper

252 100

253 51.1 24.7 37.1#

125 50.8 16.5 24.7#

