

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042723\
 Data File : BM039719.D
 Acq On : 27 Apr 2023 23:11
 Operator : CG/JU
 Sample : 02417-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW8X5

Quant Time: Apr 28 02:35:37 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 28 02:30:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.804	152	4252	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.600	136	15644	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.451	164	8988	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.204	188	19169	0.400	ng/ul	-0.01
17) Chrysene-d12	21.401	240	14978	0.400	ng/ul	0.00
23) Perylene-d12	23.745	264	12559	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.188	96	11864	1.893	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.212	152	2775	0.138	ng/ul	0.00
18) Fluoranthene-d10	19.238	212	6738	0.167	ng/ul	0.00
Target Compounds						
26) Benzo(a)pyrene	23.584	252	1671	0.042	ng/ul#	Qvalue 4


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042723\
Data File : BM039719.D
Acq On : 27 Apr 2023 23:11
Operator : CG/JU
Sample : 02417-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW8X5


Quant Time: Apr 28 02:35:37 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:30:02 2023
Response via : Initial Calibration

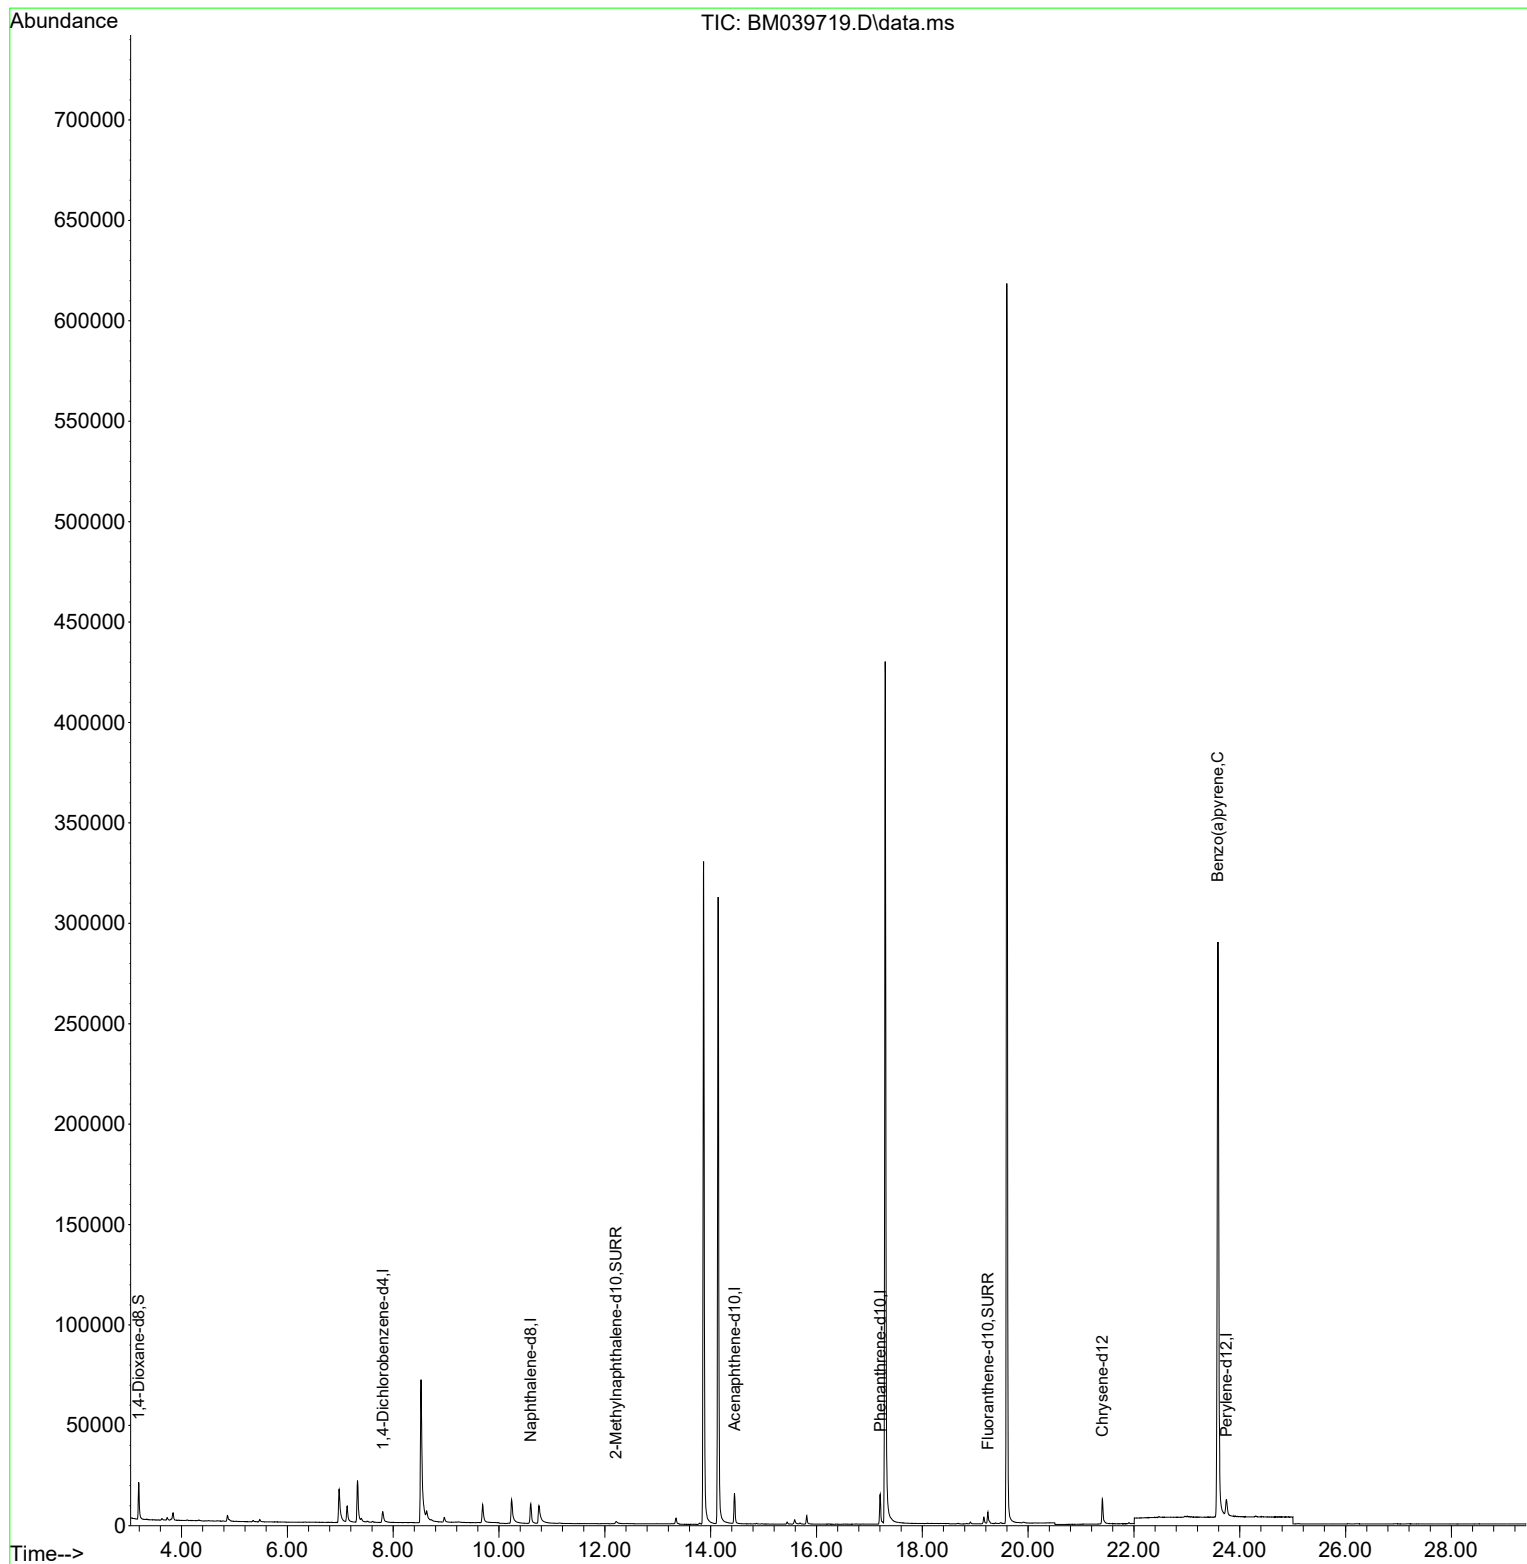

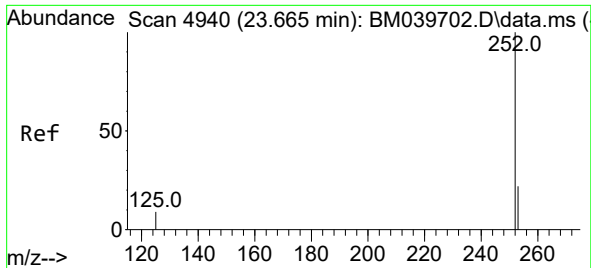

#26
Benzo(a)pyrene
Concen: 0.042 ng/ul
RT: 23.584 min Scan# 4912
Delta R.T. -0.080 min
Lab File: BM039719.D
Acq: 27 Apr 2023 23:11

Instrument :
BNA_M
ClientSampleId :
EW8X5

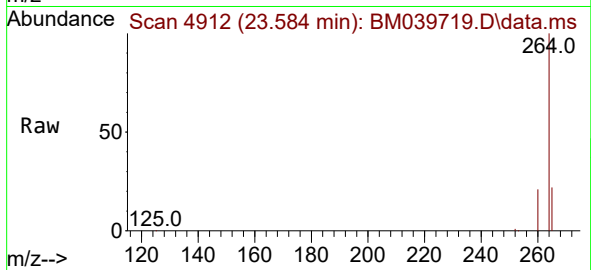

Tgt Ion:252 Resp: 1671
Ion Ratio Lower Upper
252 100
253 77.8 24.7 37.1#
125 72.6 16.5 24.7#

