

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042723\
 Data File : BM039737.D
 Acq On : 28 Apr 2023 15:43
 Operator : CG/JU
 Sample : PB152401BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK401

Quant Time: Apr 29 02:24:40 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 28 02:30:02 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.800	152	3274	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.595	136	12682	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.451	164	7237	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.204	188	16198	0.400	ng/ul	-0.01
17) Chrysene-d12	21.410	240	12766	0.400	ng/ul	0.00
23) Perylene-d12	23.754	264	12358	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.184	96	28858	5.981	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.217	152	5842	0.359	ng/ul	0.00
18) Fluoranthene-d10	19.238	212	13929	0.405	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.601	202	2113	0.043	ng/ul#	1
26) Benzo(a)pyrene	23.590	252	3966	0.102	ng/ul#	60


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042723\
Data File : BM039737.D
Acq On : 28 Apr 2023 15:43
Operator : CG/JU
Sample : PB152401BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK401

Quant Time: Apr 29 02:24:40 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 28 02:30:02 2023
Response via : Initial Calibration

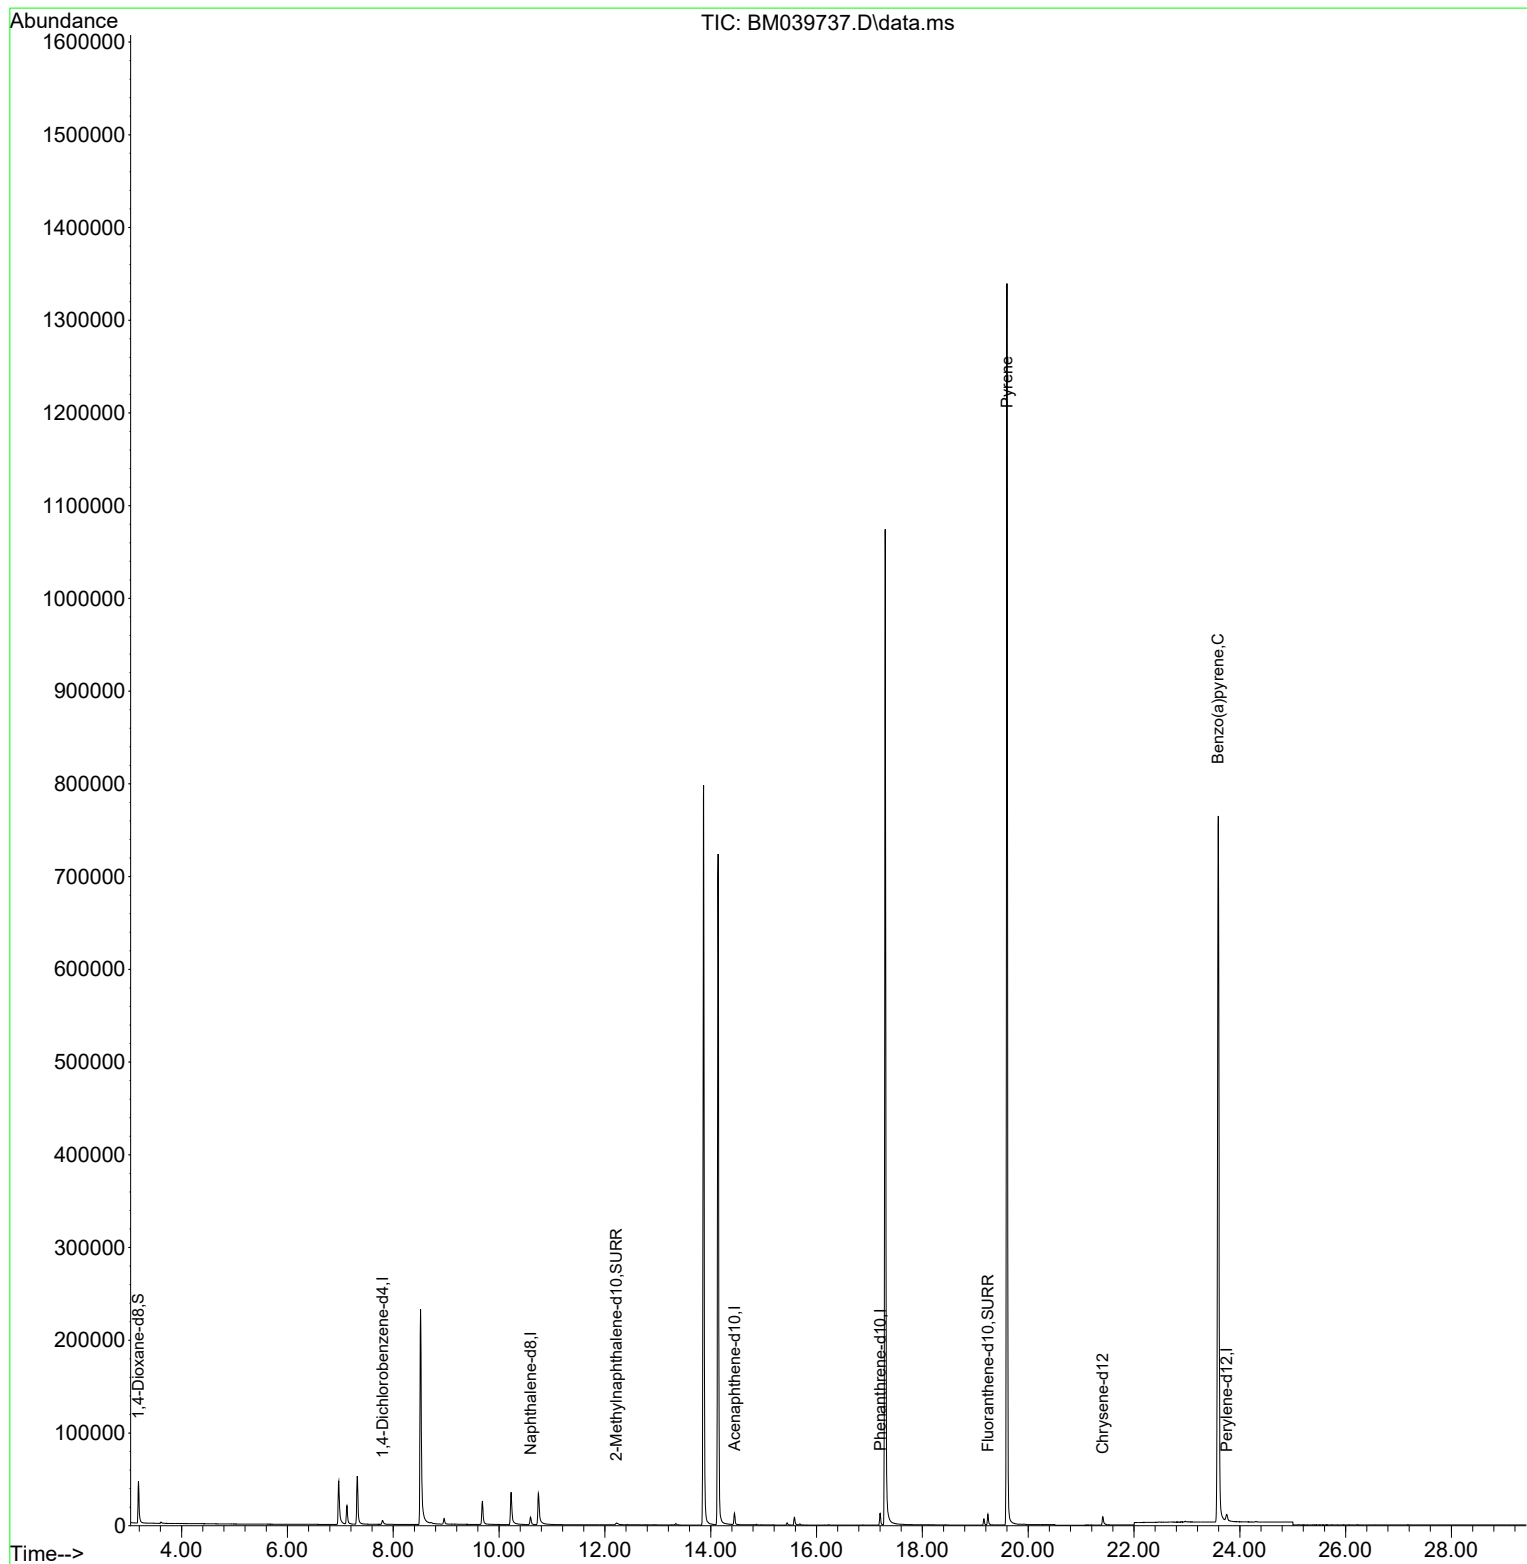

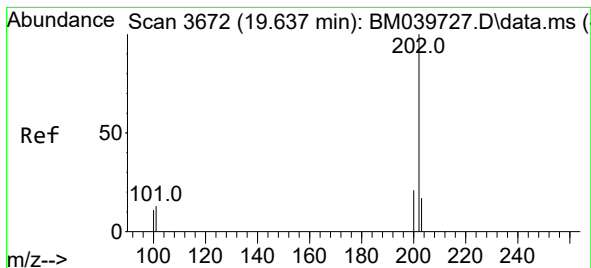

#20

Pyrene

Concen: 0.043 ng/ul

RT: 19.601 min Scan# 3

Delta R.T. -0.042 min

Lab File: BM039737.D

Acq: 28 Apr 2023 15:43

Instrument :

BNA_M

ClientSampleId :

SBLK401





Tgt Ion:202 Resp: 2113

Ion Ratio Lower Upper

202 100

101 159.1 10.9 16.3#

100 1186.5 8.9 13.3#

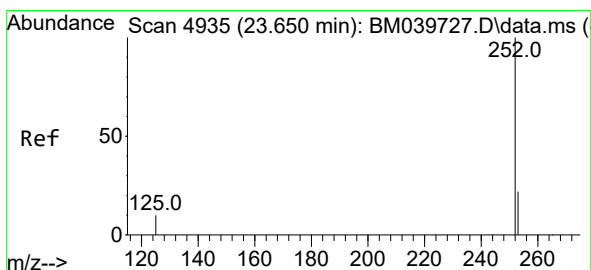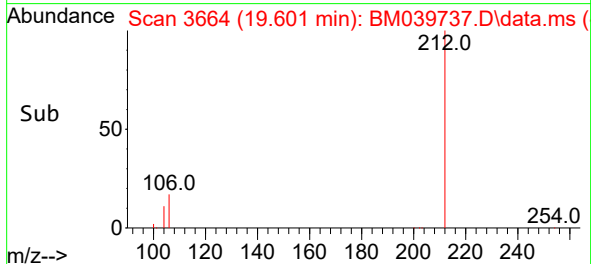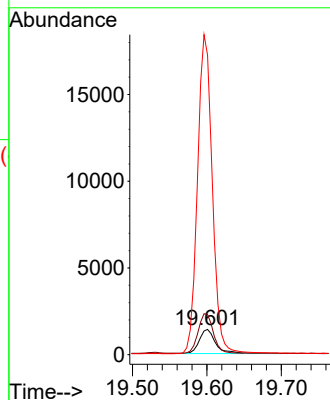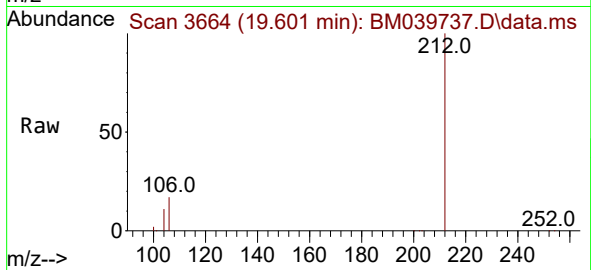

#26

Benzo(a)pyrene

Concen: 0.102 ng/ul

RT: 23.590 min Scan# 4914

Delta R.T. -0.074 min

Lab File: BM039737.D

Acq: 28 Apr 2023 15:43

Tgt Ion:252 Resp: 3966

Ion Ratio Lower Upper

252 100

253 49.6 24.7 37.1#

125 42.8 16.5 24.7#

