

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042816\
 Data File : BM005121.D
 Acq On : 28 Apr 2016 19:39
 Operator : UM/SJ
 Sample : H2639-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7N7

Quant Time: Apr 29 02:23:52 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 29 02:20:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	39850	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	191643	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	122751	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	277558	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	250939	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	207120	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	1475	1.88	ng/uL	0.00
5) Phenol-d5	6.96	99	36149	10.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	47871	25.52	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	60749	23.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	55652	19.91	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	33592	25.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	39731	26.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	73180	26.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	645	0.20	ng/ul	0.04
43) Dimethylphthalate-d6	13.84	166	252972	26.09	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	288324	24.97	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	16094	9.50	ng/ul	0.00
57) Fluorene-d10	15.42	176	212669	24.96	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	40543	25.68	ng/ul	0.00
70) Anthracene-d10	17.27	188	321982	25.87	ng/ul	0.00
76) Pyrene-d10	19.57	212	342450	29.98	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	242168	26.10	ng/ul	0.00


Target Compounds					Qvalue
17) Hexachloroethane	8.96	117	1524	1.43 ng/ul#	3


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042816\
Data File : BM005121.D
Acq On : 28 Apr 2016 19:39
Operator : UM/SJ
Sample : H2639-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7N7

Quant Time: Apr 29 02:23:52 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 29 02:20:37 2016
Response via : Initial Calibration

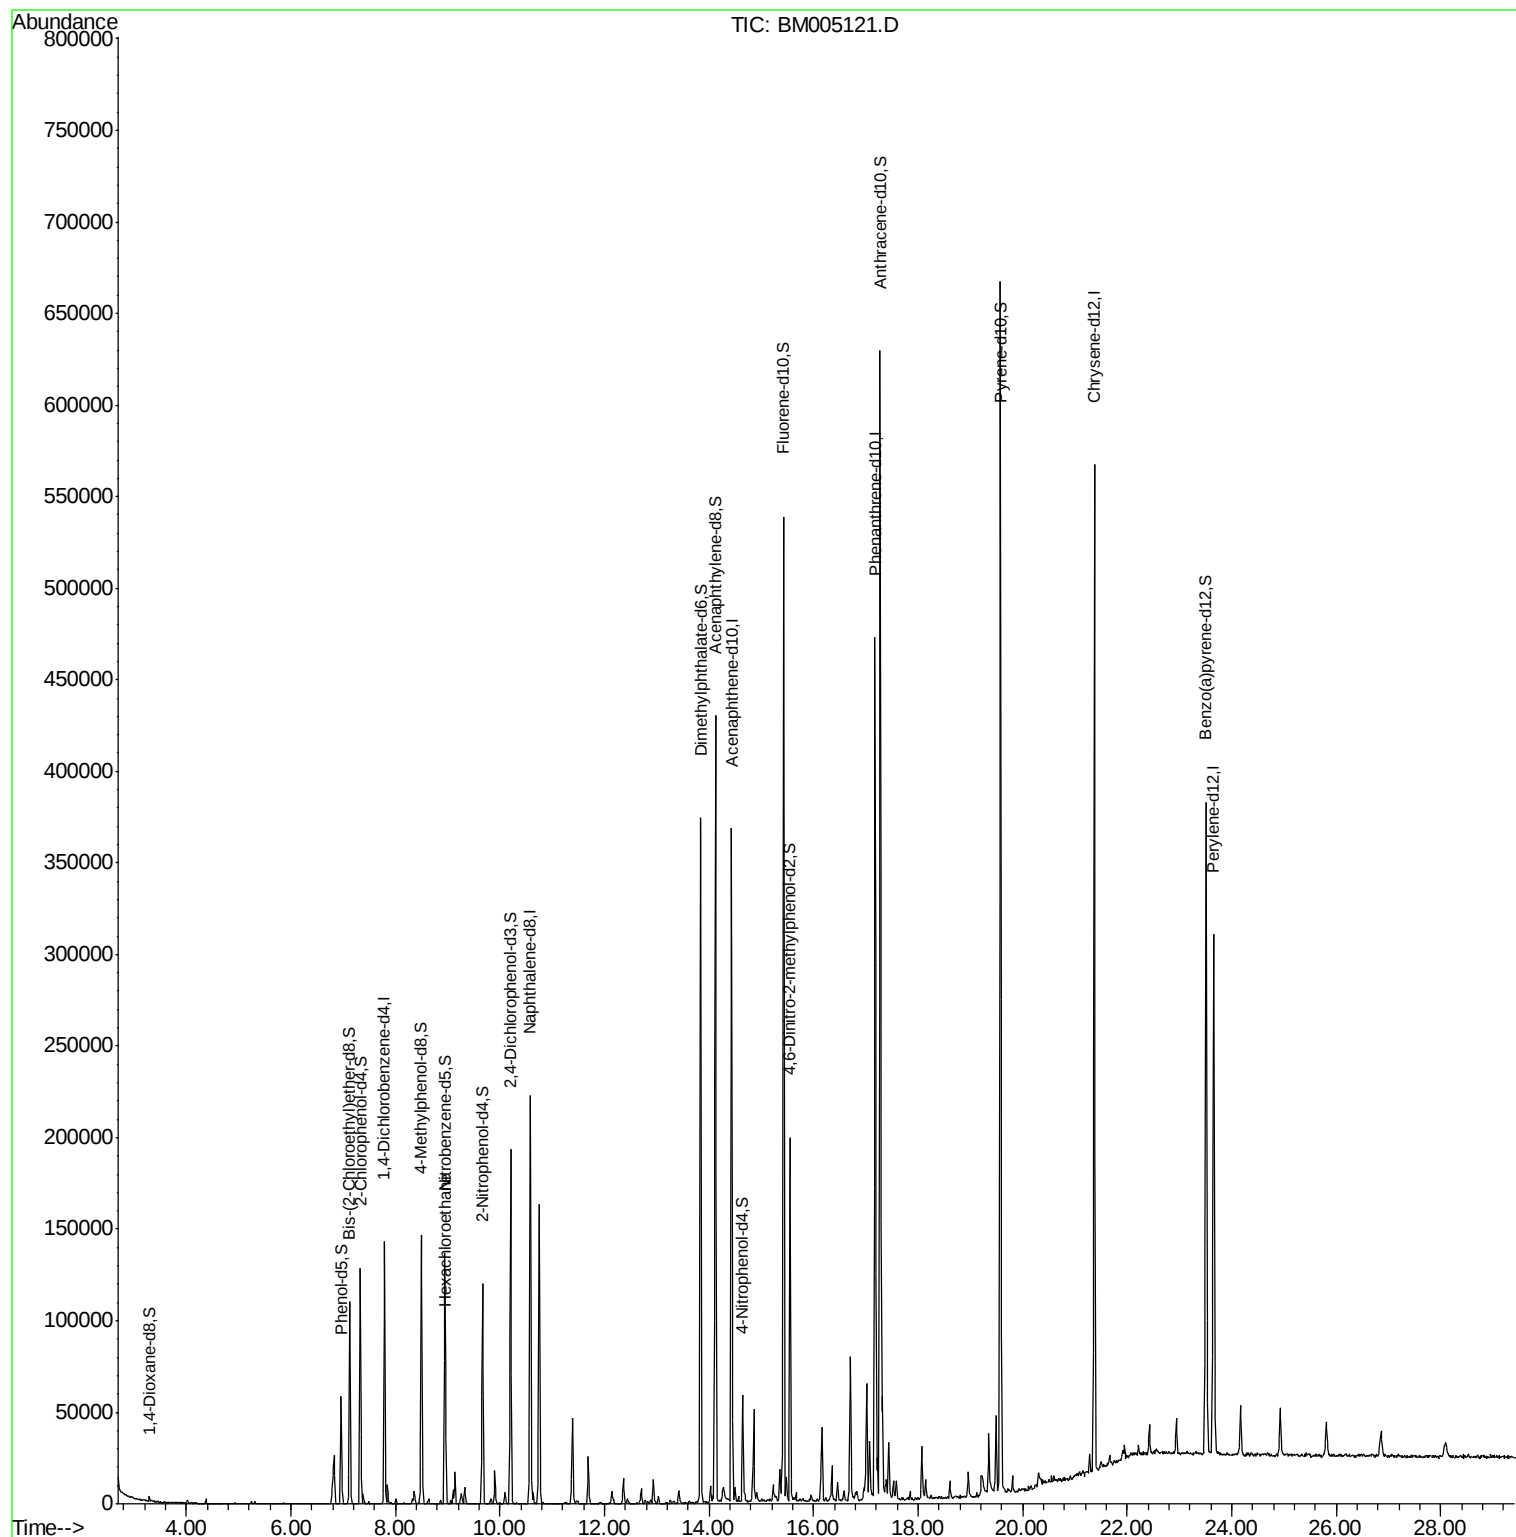

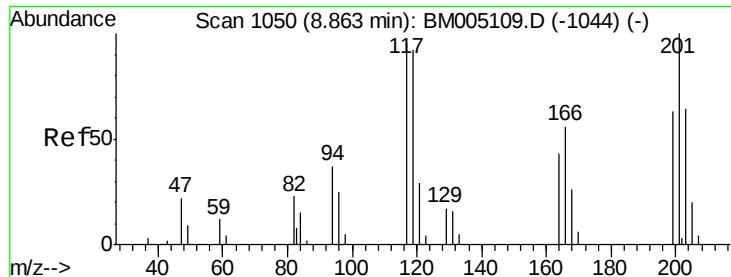

#17
 Hexachloroethane
 Concen: 1.43 ng/ul
 RT: 8.96 min Scan# 1067
 Delta R.T. 0.10 min
 Lab File: BM005121.D
 Acq: 28 Apr 2016 19:39

Instrument :
 BNA_M
 ClientSampleId :
 BC7N7

Tgt Ion:117 Resp: 1524
 Ion Ratio Lower Upper
 117 100
 201 0.0 88.5 132.7#
 199 0.0 55.4 83.2#

