

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042816\
 Data File : BM005123.D
 Acq On : 28 Apr 2016 20:52
 Operator : UM/SJ
 Sample : H2639-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7N5

Quant Time: Apr 29 11:25:08 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 29 02:20:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	39338	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	185859	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	121184	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	287829	20.00	ng/ul	0.00
75) Chrysene-d12	21.37	240	320785	20.00	ng/ul	0.00
83) Perylene-d12	23.65	264	279648	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	854	1.10	ng/uL	0.00
5) Phenol-d5	6.96	99	21411	6.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	52736	28.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	58319	22.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	42637	15.45	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	37337	29.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	43227	30.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	74922	27.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.73	131	281	0.09	ng/ul	0.01
43) Dimethylphthalate-d6	13.84	166	319249	33.36	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	338148	29.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.64	143	12071	7.22	ng/ul	0.00
57) Fluorene-d10	15.42	176	266735	31.72	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	56224	34.34	ng/ul	0.00
70) Anthracene-d10	17.27	188	450525	34.91	ng/ul	0.00
76) Pyrene-d10	19.57	212	512099	35.07	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.51	264	433863	34.63	ng/ul	0.00


Target Compounds						Ovalue
69) Phenanthrene	17.22	178	29428	1.92	ng/ul	98
72) Carbazole	17.58	167	14228	1.07	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042816\
Data File : BM005123.D
Acq On : 28 Apr 2016 20:52
Operator : UM/SJ
Sample : H2639-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7N5

Quant Time: Apr 29 11:25:08 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 29 02:20:37 2016
Response via : Initial Calibration

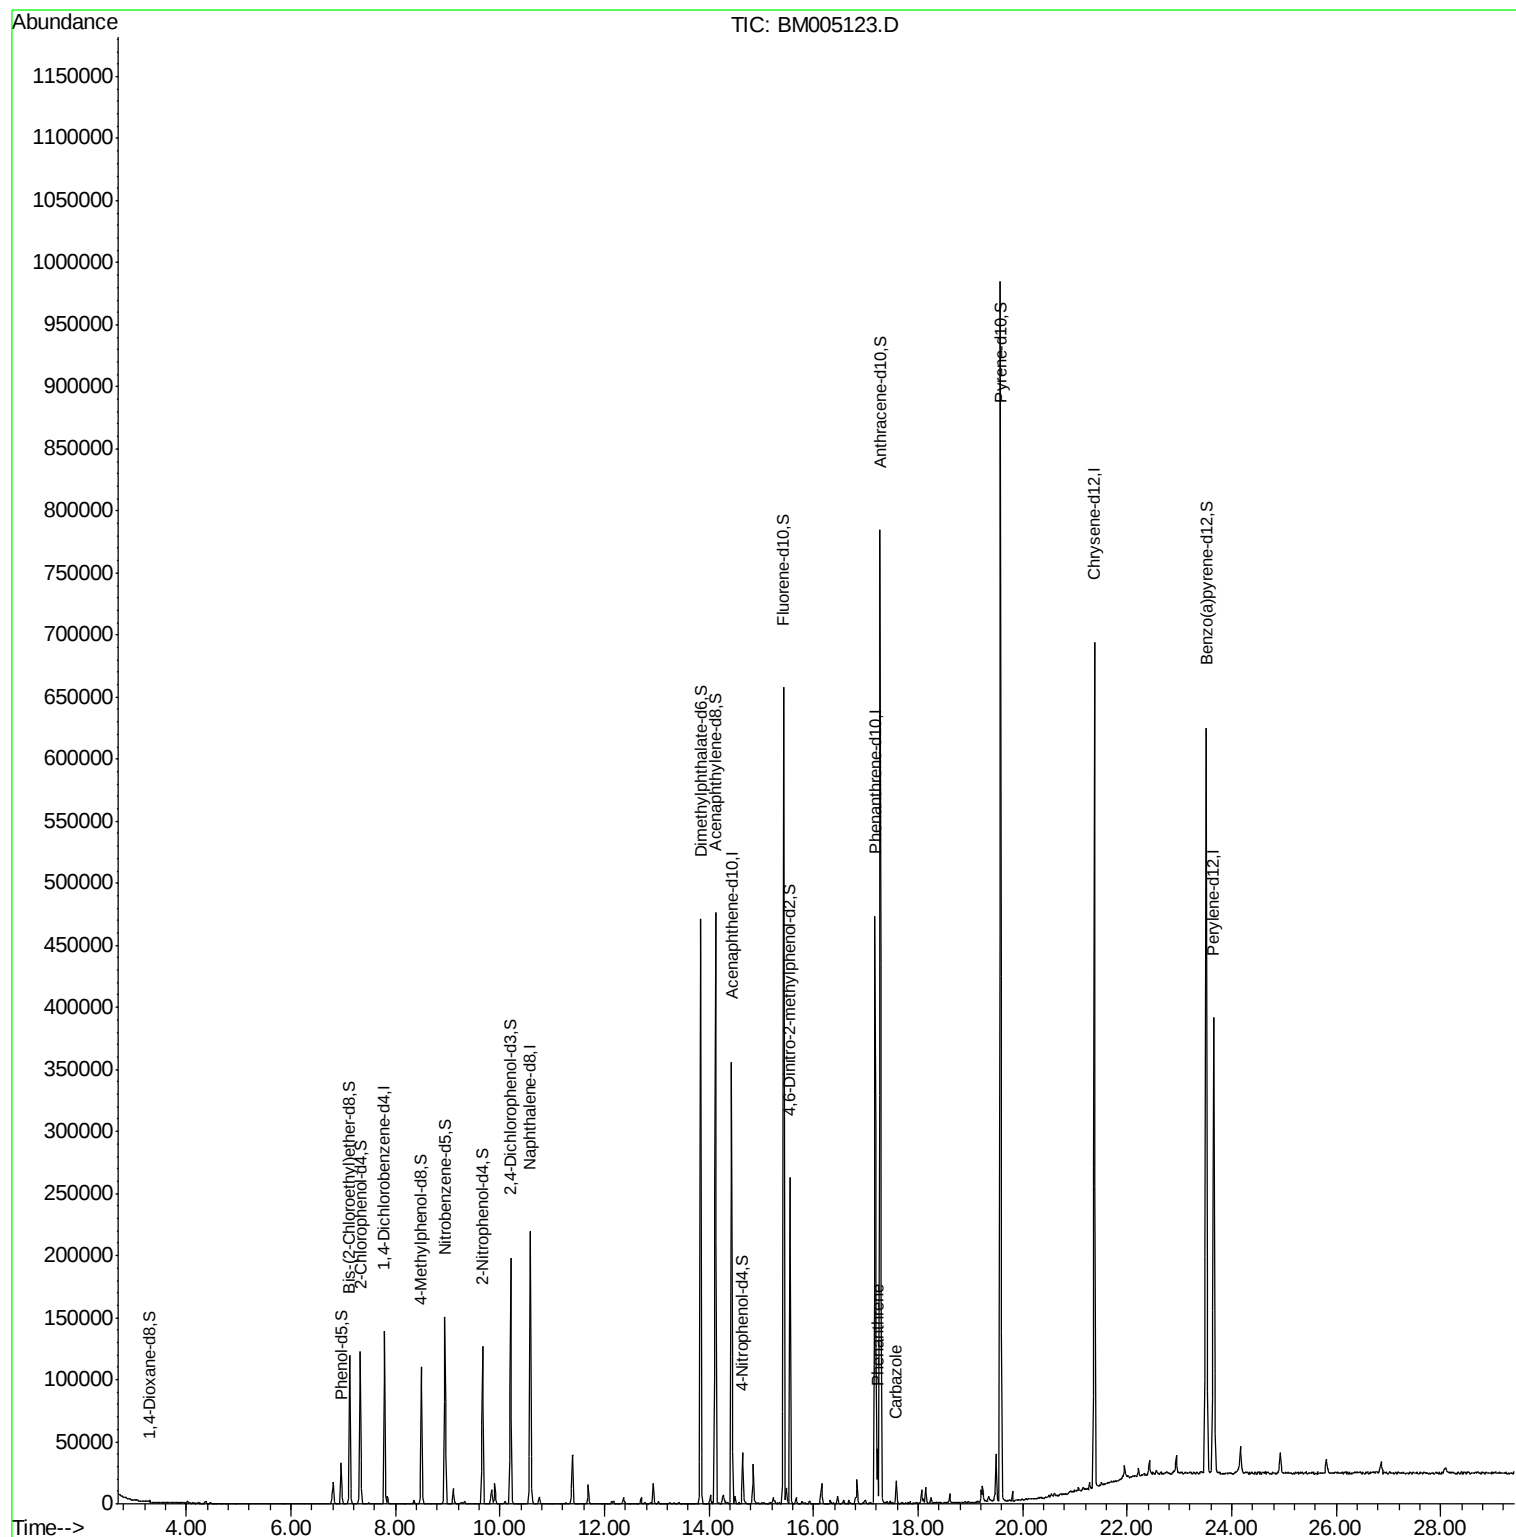

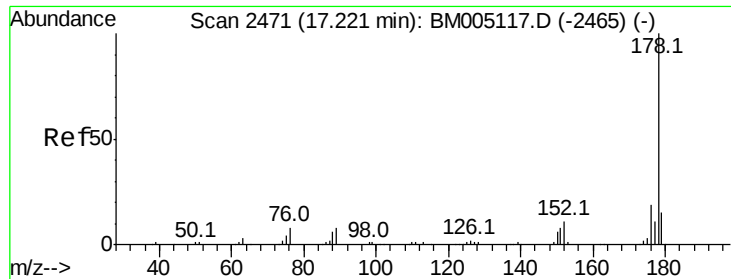

#69

Phenanthrene

Concen: 1.92 ng/ul

RT: 17.22 min Scan# 2470

Delta R.T. -0.01 min

Lab File: BM005123.D

Acq: 28 Apr 2016 20:52

Instrument :

BNA_M

ClientSampleId :

BC7N5


Tot Ion:178 Resp: 29428

Ion Ratio Lower Upper

178 100

179 16.0 11.8 17.8




176 18.1 15.2 22.8

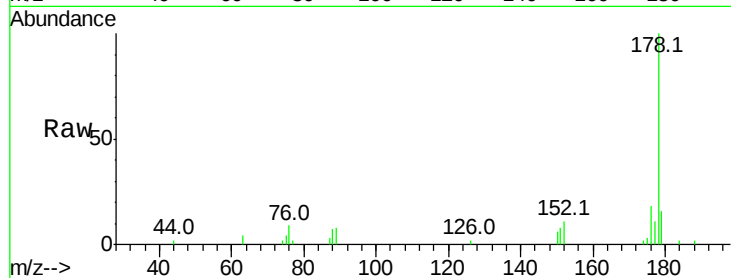

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

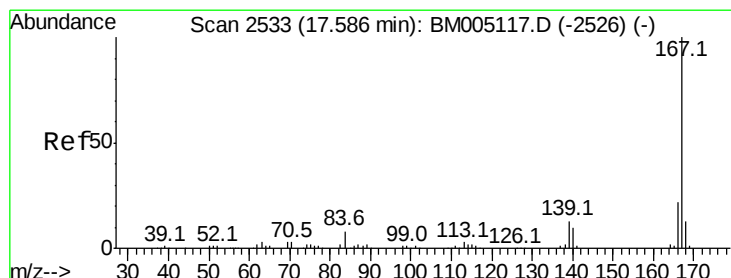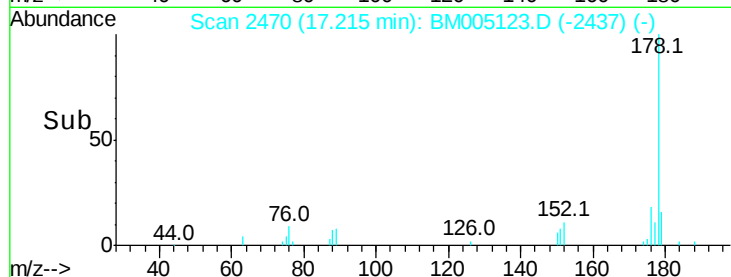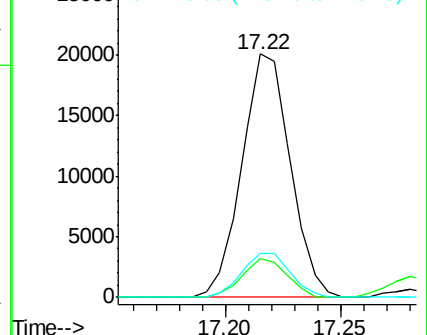

#72

Carbazole

Concen: 1.07 ng/ul

RT: 17.58 min Scan# 2532

Delta R.T. -0.01 min

Lab File: BM005123.D

Acq: 28 Apr 2016 20:52


Tgt Ion:167 Resp: 14228

Ion Ratio Lower Upper

167 100

166 21.3 16.6 25.0

139 13.1 10.2 15.4

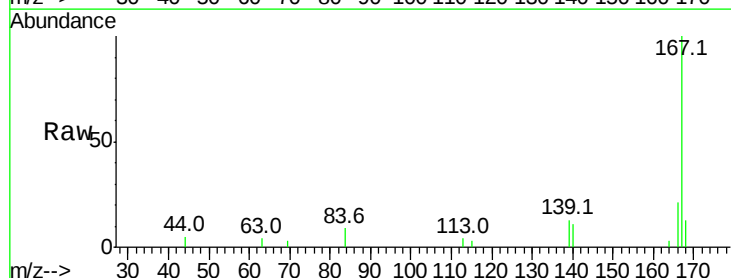

Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

