

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042816\
 Data File : BM005130.D
 Acq On : 29 Apr 2016 01:05
 Operator : UM/SJ
 Sample : H2639-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7K2

Manual Integrations
 APPROVED

sohil
 4/29/2016 10:36:39 AM

Quant Time: Apr 29 05:25:15 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 29 02:20:37 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	40493	20.00	ng/ul	0.00
18) Naphthalene-d8	10.57	136	194141	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.43	164	125474	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.17	188	292940	20.00	ng/ul	0.00
75) Chrysene-d12	21.36	240	284397	20.00	ng/ul	-0.01
83) Perylene-d12	23.64	264	233567	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	4074	5.11	ng/uL	0.00
5) Phenol-d5	6.96	99	90880	27.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	54095	28.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.32	132	71065	26.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.49	113	79362	27.95	ng/ul	0.00
19) Nitrobenzene-d5	8.95	128	36743	27.33	ng/ul	0.00
22) 2-Nitrophenol-d4	9.66	143	43101	28.73	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.20	165	77885	27.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.72	131	134262	40.20	ng/ul	0.00
43) Dimethylphthalate-d6	13.84	166	285004	28.76	ng/ul	0.00
46) Acenaphthylene-d8	14.12	160	331124	28.06	ng/ul	0.00
51) 4-Nitrophenol-d4	14.63	143	46145m	26.64	ng/ul	0.00
57) Fluorene-d10	15.42	176	246094	28.26	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.54	200	35833	21.51	ng/ul	0.00
70) Anthracene-d10	17.27	188	394013	30.00	ng/ul	0.00
76) Pyrene-d10	19.57	212	437210	33.77	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.50	264	322489	30.82	ng/ul	-0.01

Target Compounds

						Ovalue
28) Naphthalene	10.63	128	32756	3.35	ng/ul	99
34) 2-Methylnaphthalene	12.24	142	11807	1.63	ng/ul	98
44) Dimethylphthalate	13.88	163	75276	7.57	ng/ul	99
49) Acenaphthene	14.49	153	9359	1.14	ng/ul	98
53) Dibenzofuran	14.83	168	12751	1.05	ng/ul	98
58) Fluorene	15.48	166	9866	1.05	ng/ul	94
69) Phenanthrene	17.22	178	53410	3.43	ng/ul	99
74) Fluoranthene	19.23	202	32402	1.89	ng/ul	99
77) Pvrene	19.60	202	22911	1.39	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM042816\
Data File : BM005130.D
Acq On : 29 Apr 2016 01:05
Operator : UM/SJ
Sample : H2639-15
Misc :
ALS Vial : 21 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BC7K2

Manual Integrations
APPROVED

sohil
4/29/2016 10:36:39 AM

Quant Time: Apr 29 05:25:15 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 29 02:20:37 2016
Response via : Initial Calibration

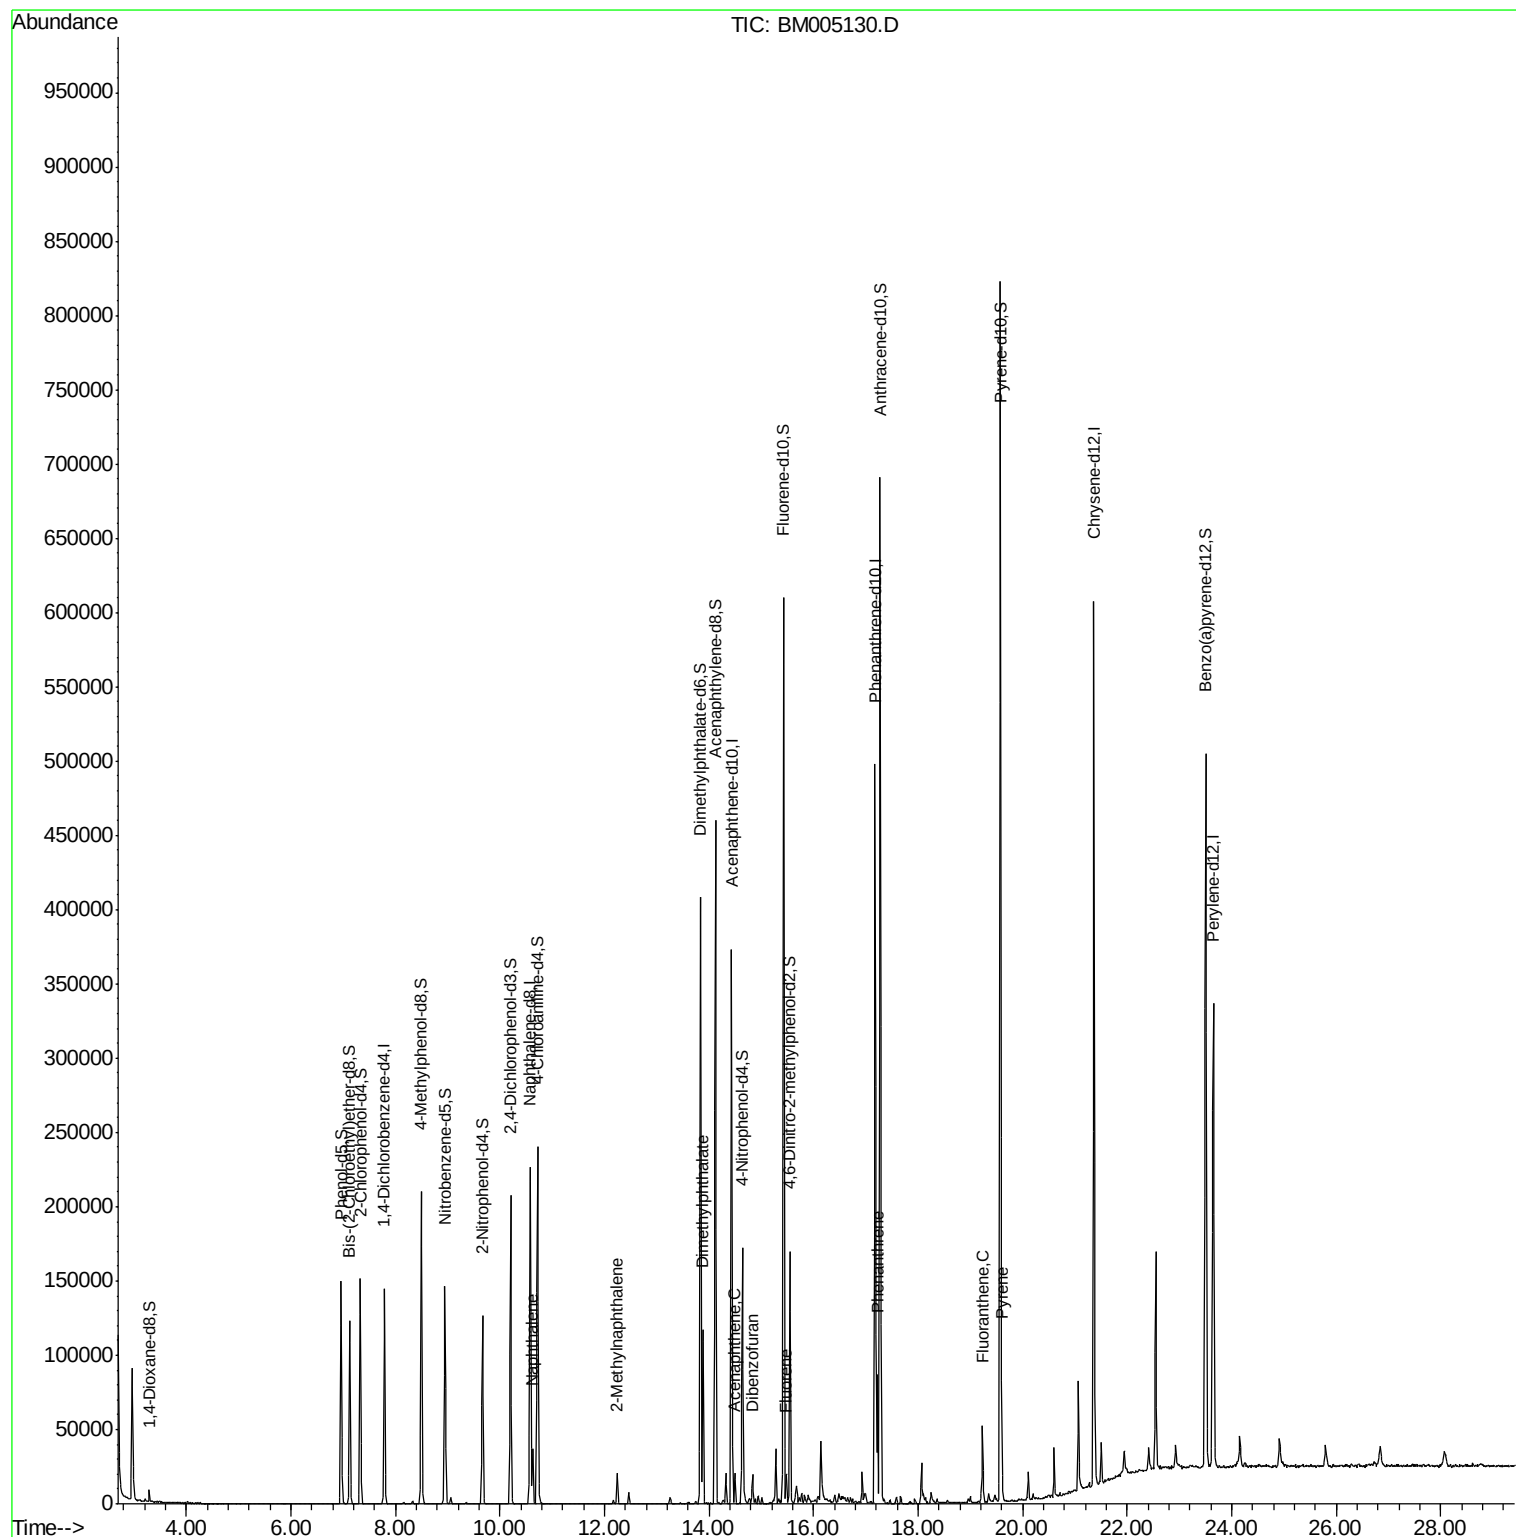

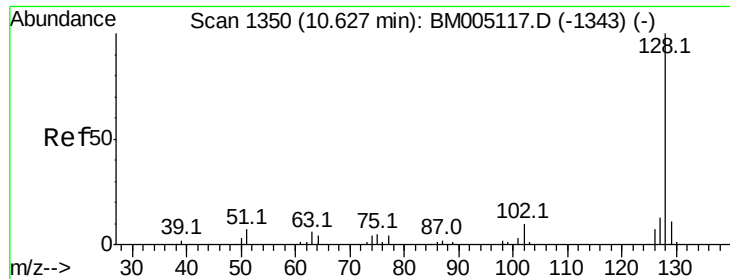


#28
Naphthalene
Concen: 3.35 ng/ul
RT: 10.63 min Scan# 1350
Delta R.T. -0.00 min
Lab File: BM005130.D
Acq: 29 Apr 2016 01:05

Instrument :
BNA_M
ClientSampled :
BC7K2

Tot Ion	Ratio	Lower	Upper
128	100		
129	10.8	8.7	13.1
127	12.8	10.6	15.8

Manual Integrations
APPROVED

sohil
4/29/2016 10:36:39 AM



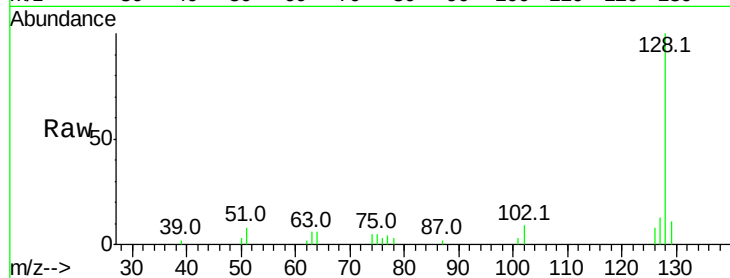


Abundance

Ion 128.00 (127.70 to 128.70): E


Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

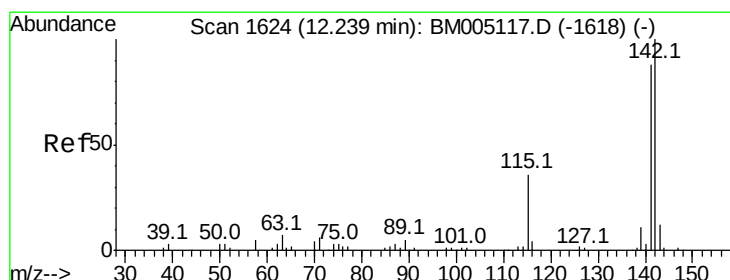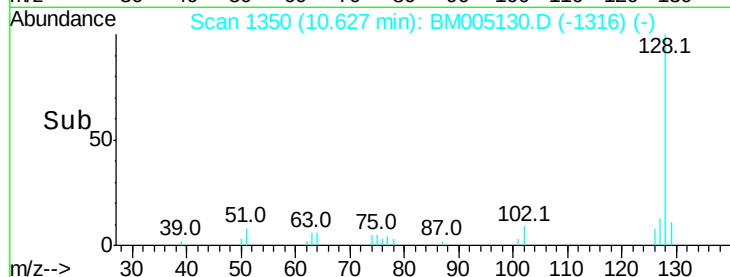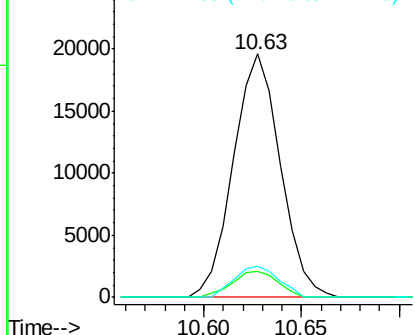

#34
2-Methylnaphthalene
Concen: 1.63 ng/ul
RT: 12.24 min Scan# 1624
Delta R.T. -0.01 min
Lab File: BM005130.D
Acq: 29 Apr 2016 01:05



Tgt Ion	Ratio	Lower	Upper
142	100		
141	86.1	70.3	105.5

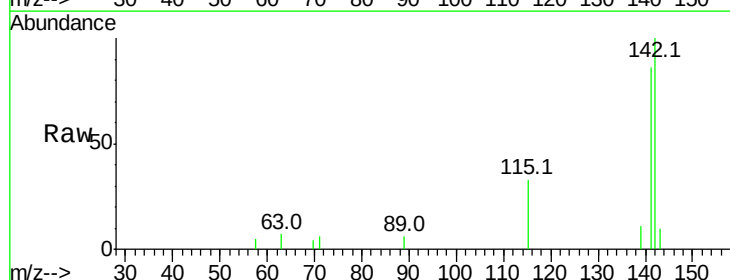


Abundance

Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

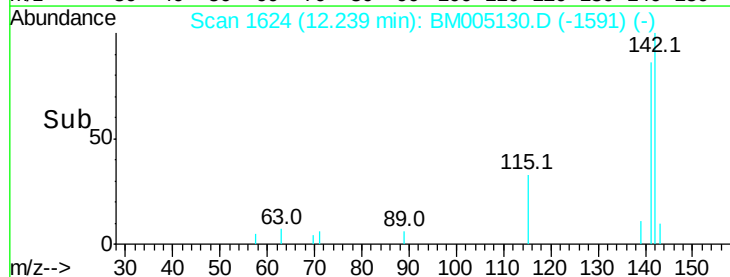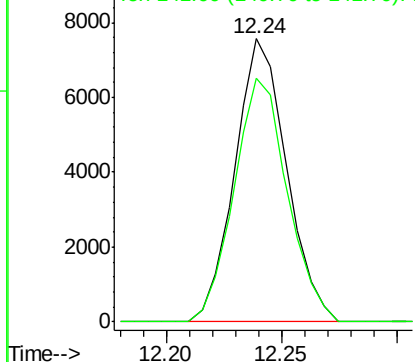

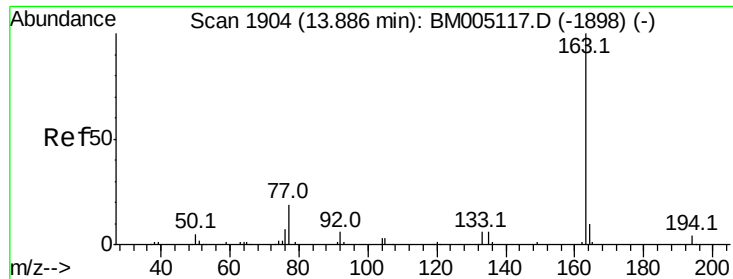

#44

Dimethylphthalate

Concen: 7.57 ng/ul

RT: 13.88 min Scan# 1903

Delta R.T. -0.01 min

Lab File: BM005130.D

Acq: 29 Apr 2016 01:05

Instrument :

BNA_M





ClientSampleId :

BC7K2

Tot Ion:	163	Resp:	75276
Ion Ratio	Lower	Upper	
163	100		
194	3.9	3.3	4.9
164	10.4	8.2	12.2

Manual Integrations
APPROVED

sohil
4/29/2016 10:36:39 AM

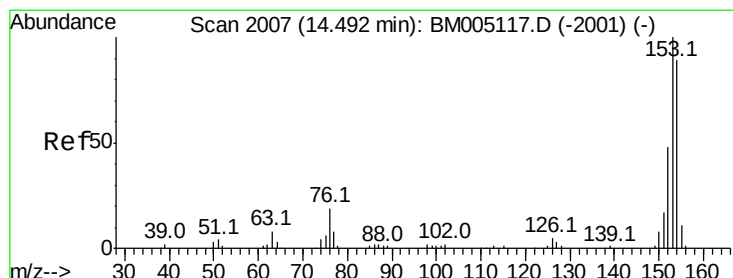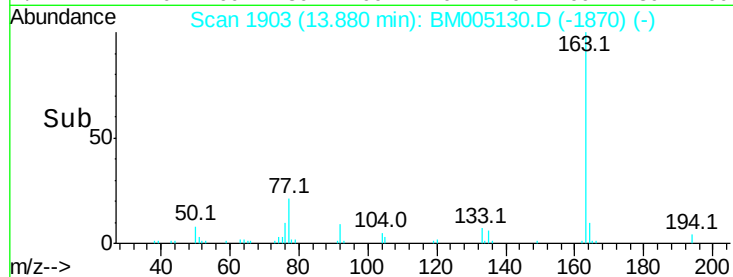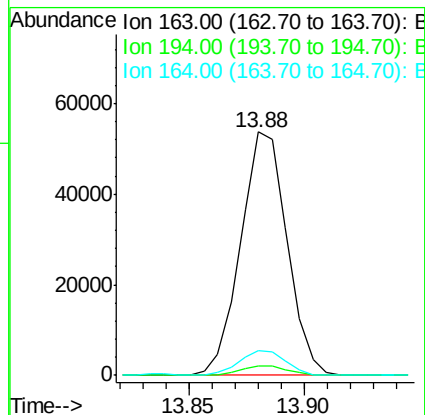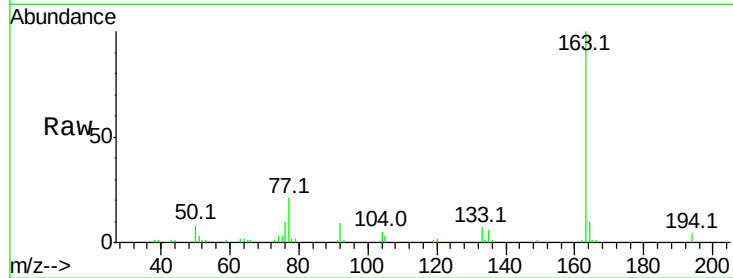

#49

Acenaphthene

Concen: 1.14 ng/ul




RT: 14.49 min Scan# 2007


Delta R.T. -0.01 min

Lab File: BM005130.D

Acq: 29 Apr 2016 01:05

Tgt Ion:	153	Resp:	9359
Ion Ratio	Lower	Upper	
153	100		
152	47.2	37.7	56.5
154	92.3	71.4	107.2

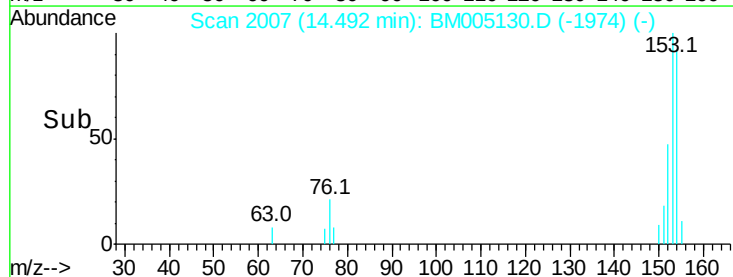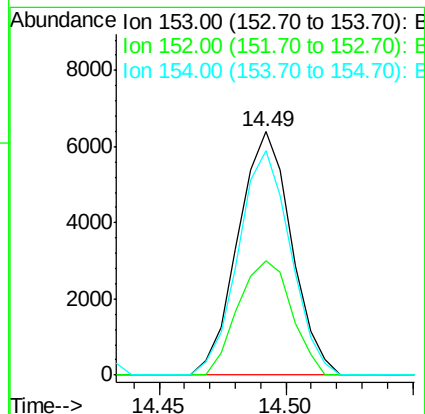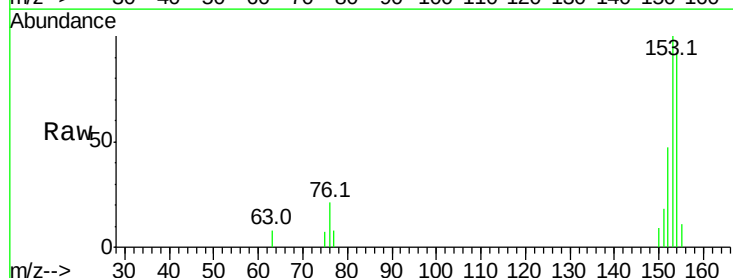

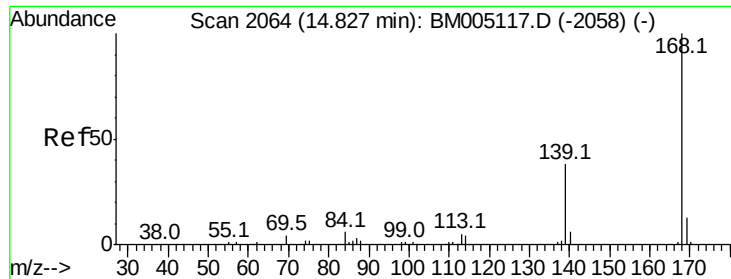

#53

Dibenzenofuran

Concen: 1.05 ng/ul

RT: 14.83 min Scan# 2064

Delta R.T. -0.01 min

Lab File: BM005130.D

Acq: 29 Apr 2016 01:05

Instrument :

BNA_M

ClientSampleId :

BC7K2

Tot Ion:168 Resp: 12751

Ion Ratio Lower Upper


168 100

139 36.2 29.9 44.9

Manual Integrations
APPROVED

sohil

4/29/2016 10:36:39 AM

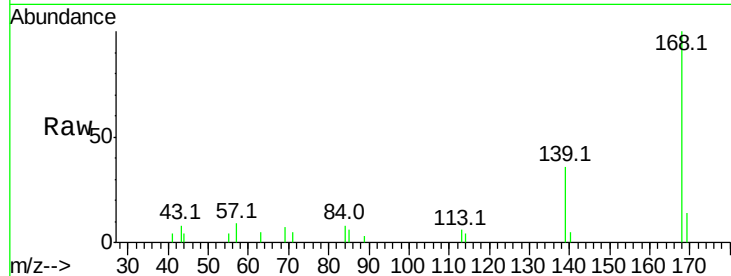

Abundance Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

14.83

10000

8000



6000

4000

2000

0

Time-->

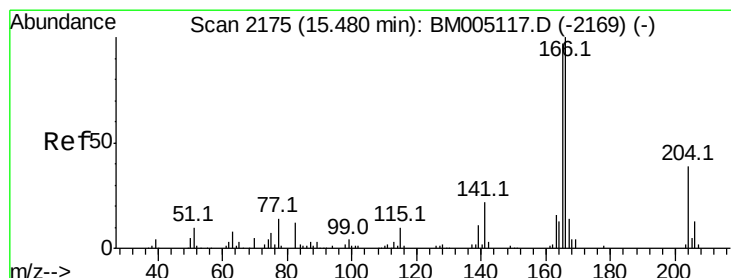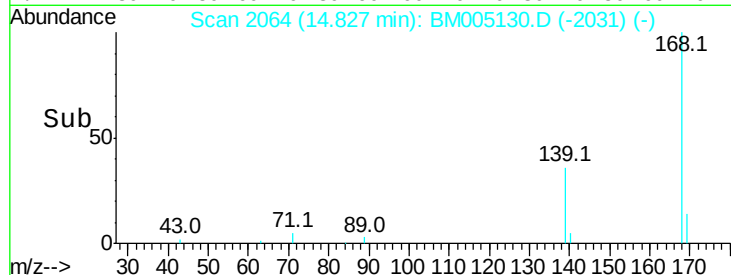

#58

Fluorene

Concen: 1.05 ng/ul

RT: 15.48 min Scan# 2175

Delta R.T. -0.00 min

Lab File: BM005130.D

Acq: 29 Apr 2016 01:05


Tgt Ion:166 Resp: 9866

Ion Ratio Lower Upper

166 100

165 90.9 77.7 116.5

167 12.5 10.9 16.3

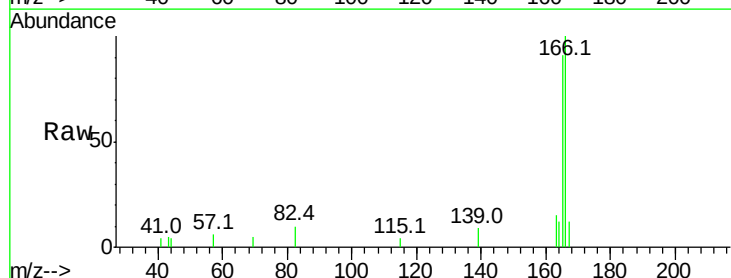

Abundance Ion 166.00 (165.70 to 166.70): E

Ion 165.00 (164.70 to 165.70): E

Ion 167.00 (166.70 to 167.70): E

15.48

8000


6000


4000

2000

0

Time-->

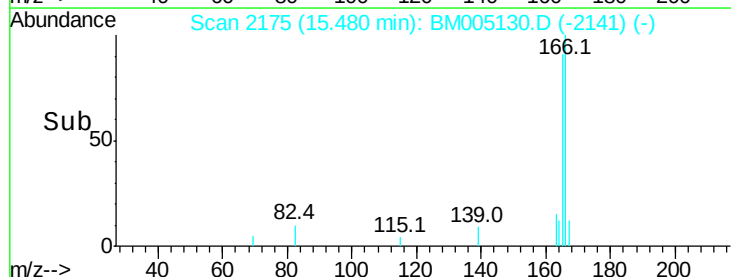

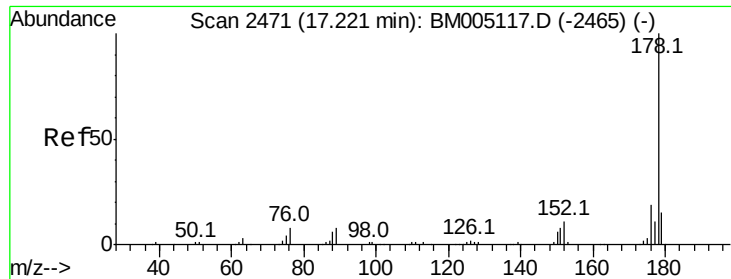





#69
 Phenanthrene
 Concen: 3.43 ng/ul
 RT: 17.22 min Scan# 2470
 Delta R.T. -0.01 min
 Lab File: BM005130.D
 Acq: 29 Apr 2016 01:05

Instrument :
 BNA_M
 ClientSampleId :
 BC7K2

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.8	11.8	17.8
176	18.8	15.2	22.8




Manual Integrations
 APPROVED


sohil
 4/29/2016 10:36:39 AM

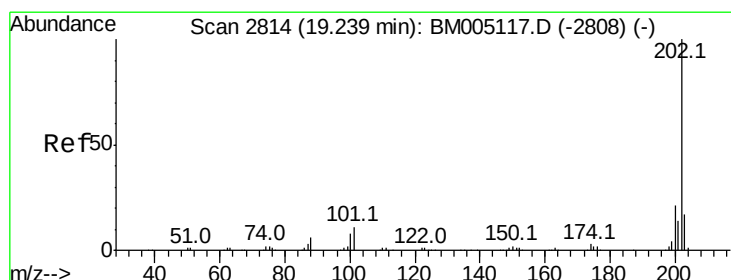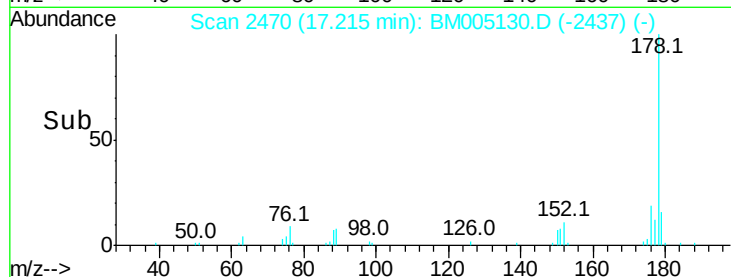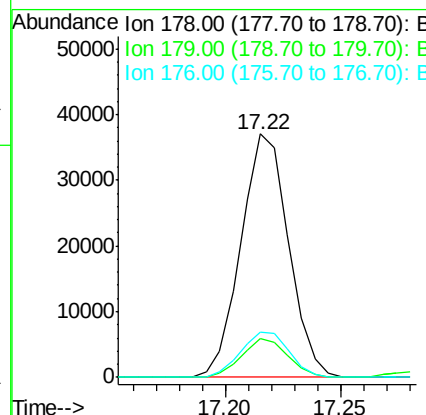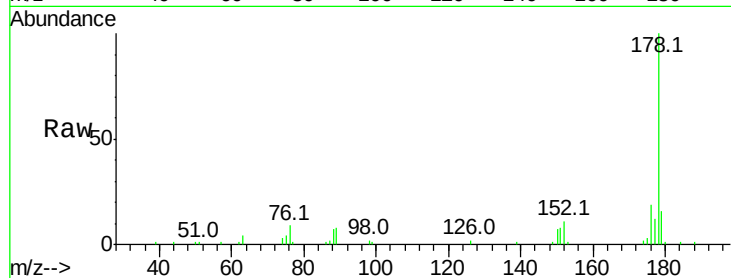

#74
 Fluoranthene
 Concen: 1.89 ng/ul
 RT: 19.23 min Scan# 2813
 Delta R.T. -0.01 min
 Lab File: BM005130.D
 Acq: 29 Apr 2016 01:05

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.0	9.0	13.4
100	8.7	6.6	10.0

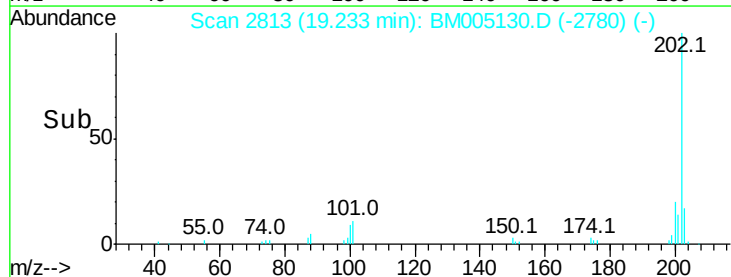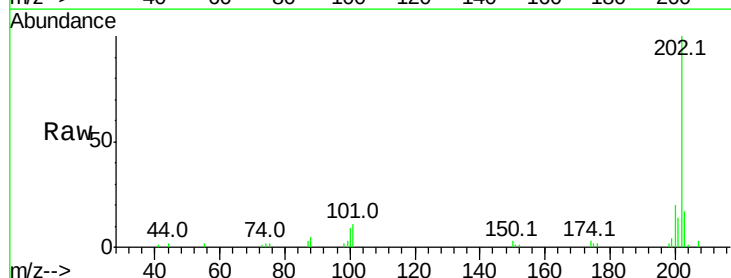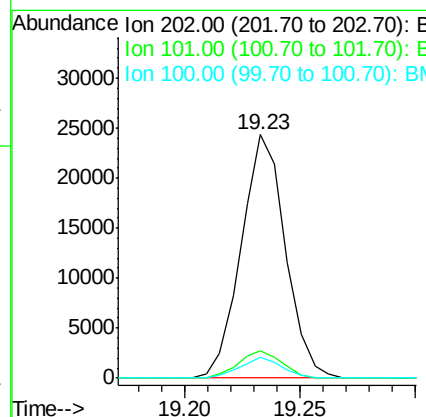

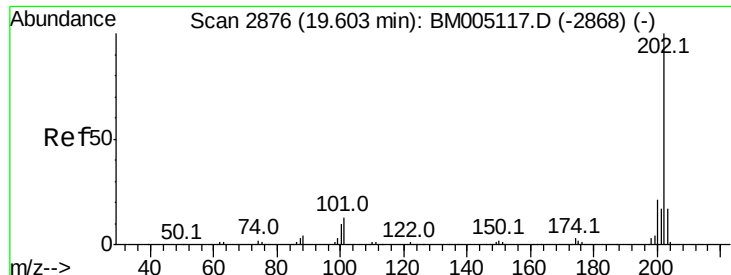


#77
 Pvrene
 Concen: 1.39 ng/ul
 RT: 19.60 min Scan# 2875
 Delta R.T. -0.01 min
 Lab File: BM005130.D
 Acq: 29 Apr 2016 01:05

Instrument :
 BNA_M
 ClientSampleId :
 BC7K2

Tot Ion:	202	Resp:	22911
Ion Ratio	Lower	Upper	
202	100		
101	13.6	10.5	15.7
100	10.3	8.2	12.2

Manual Integrations
 APPROVED

sohil
 4/29/2016 10:36:39 AM

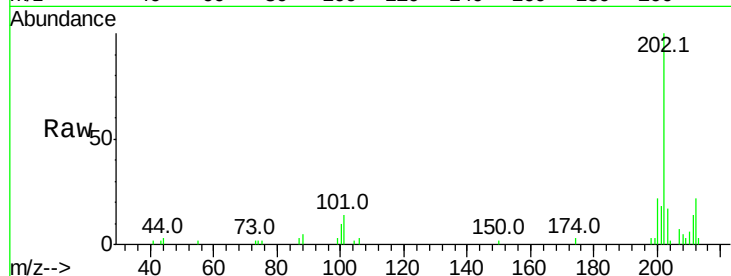

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

