

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042816\
 Data File : BM005118.D
 Acq On : 28 Apr 2016 17:50
 Operator : UM/SJ
 Sample : H2639-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BC7W1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.957	721	726	734	rBB	34406	51869	4.08%	0.480%
2	7.122	749	754	764	rBB	140454	216885	17.06%	2.008%
3	7.322	783	788	797	rBB	142109	218443	17.18%	2.022%
4	7.792	861	868	875	rBB	141530	225962	17.77%	2.092%
5	8.492	982	987	994	rBV	111792	174454	13.72%	1.615%
6	8.945	1058	1064	1073	rBV	174007	281805	22.16%	2.608%
7	9.663	1181	1186	1193	rBV	147071	237812	18.70%	2.201%
8	10.198	1271	1277	1289	rBB	204700	335815	26.41%	3.108%
9	10.575	1335	1341	1348	rBV	210200	361572	28.44%	3.347%
10	10.645	1348	1353	1358	rVB2	7998	14363	1.13%	0.133%
11	13.839	1890	1896	1902	rBV	469569	656981	51.67%	6.081%
12	14.121	1937	1944	1953	rBV	518279	750574	59.03%	6.947%
13	14.268	1962	1969	1983	rBV2	8622	19344	1.52%	0.179%
14	14.427	1990	1996	2003	rBV2	353152	538033	42.32%	4.980%
15	14.633	2025	2031	2043	rBV	25080	43432	3.42%	0.402%
16	15.427	2159	2166	2172	rBV	663134	984831	77.46%	9.116%
17	15.545	2181	2186	2193	rBV	196244	260617	20.50%	2.412%
18	17.174	2457	2463	2470	rBV2	466586	673980	53.01%	6.238%
19	17.274	2474	2480	2499	rVB2	749294	1092960	85.96%	10.117%
20	19.574	2865	2871	2883	rBV2	901098	1271486	100.00%	11.769%
21	21.368	3170	3176	3185	rBV	584157	762979	60.01%	7.062%
22	23.503	3531	3539	3548	rBV2	521200	974286	76.63%	9.018%
23	23.650	3556	3564	3577	rVB	316740	610052	47.98%	5.647%
24	24.168	3647	3652	3657	rVB4	11881	21290	1.67%	0.197%
25	24.921	3775	3780	3788	rVB3	11758	23765	1.87%	0.220%


Sum of corrected areas: 10803590

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042816\
Data File : BM005118.D
Acq On : 28 Apr 2016 17:50
Operator : UM/SJ
Sample : H2639-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7W1

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

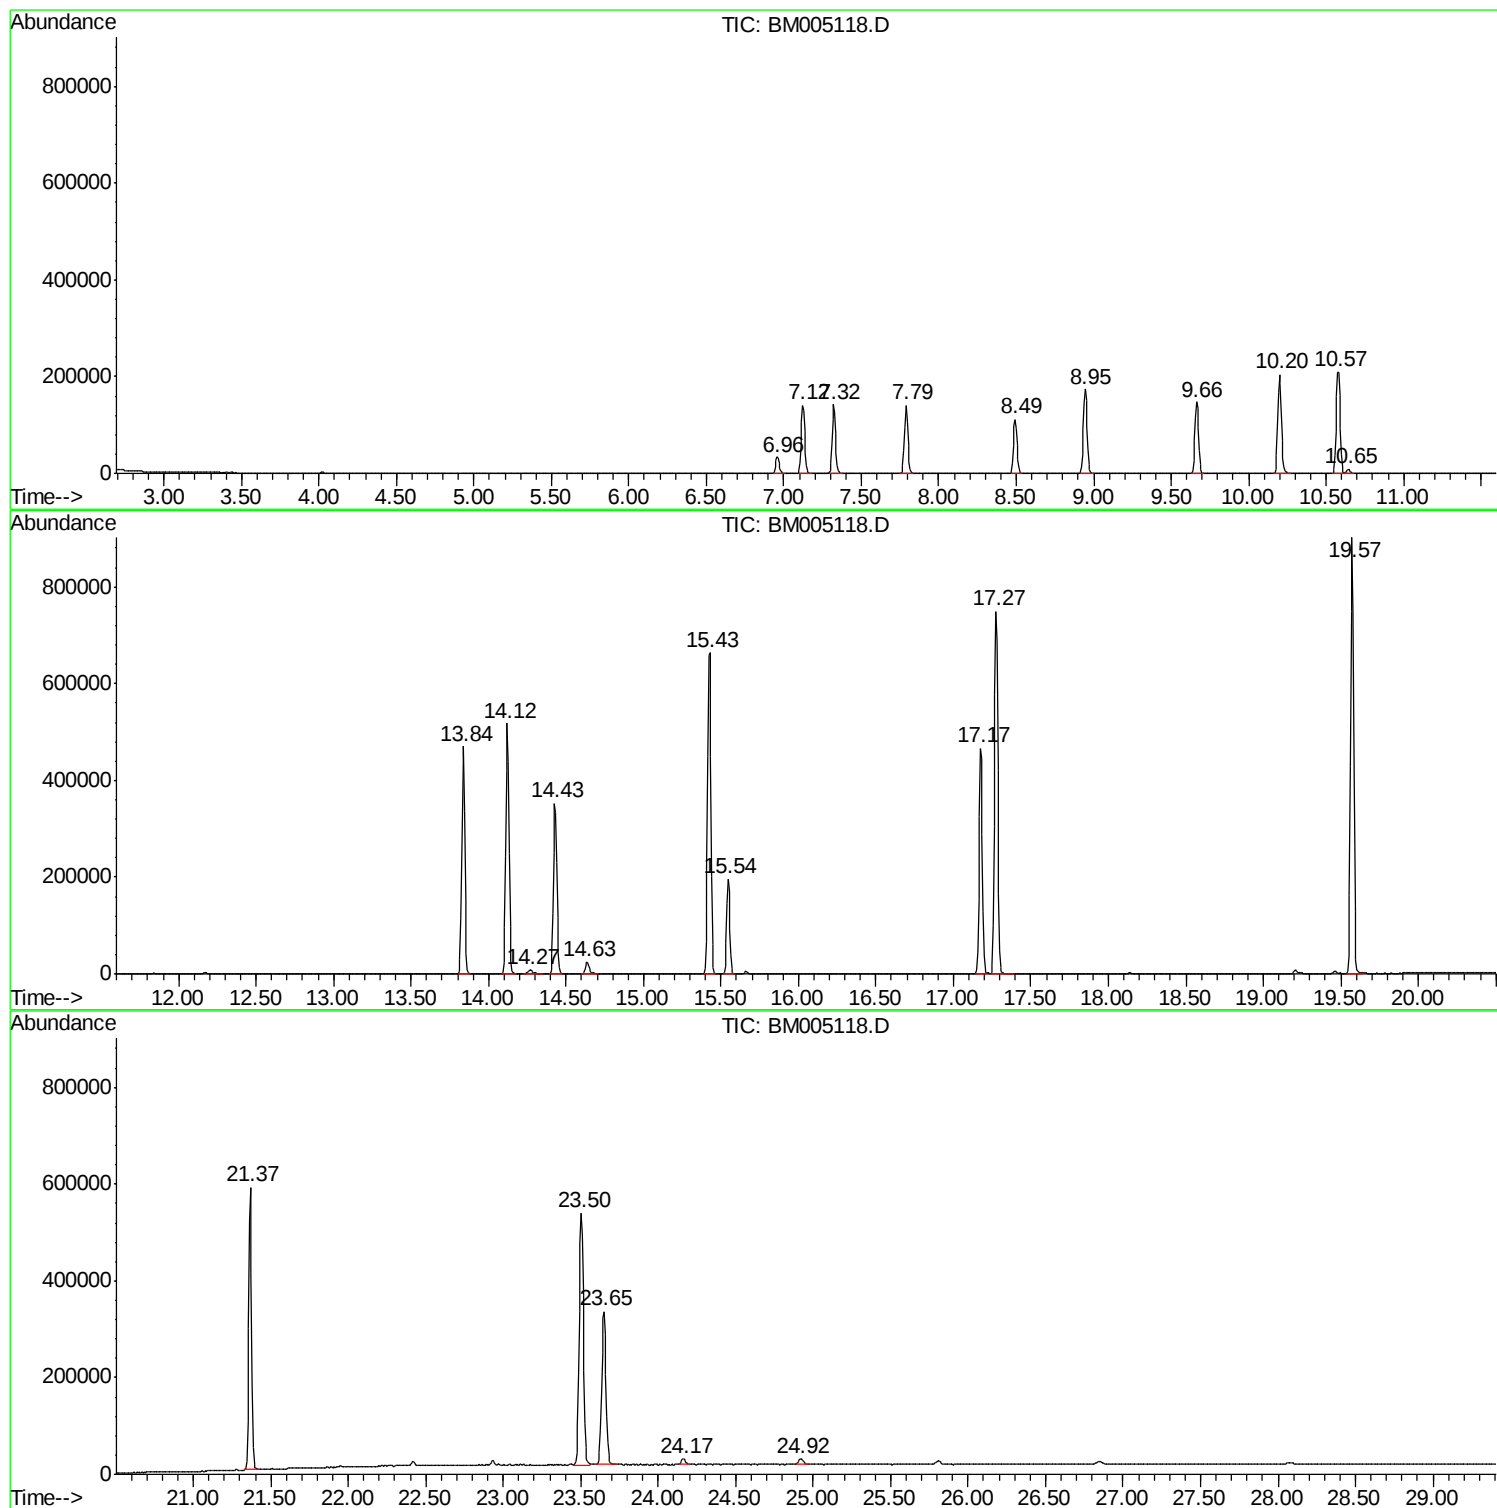

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042816\
Data File : BM005118.D
Acq On : 28 Apr 2016 17:50
Operator : UM/SJ
Sample : H2639-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7W1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM042816\
Data File : BM005118.D
Acq On : 28 Apr 2016 17:50
Operator : UM/SJ
Sample : H2639-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BC7W1

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042516.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc