

Data File : BM009790.D
Acq On : 28 Apr 2017 21:03
Operator : SJ/MA
Sample : I2845-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHT07

Quant Time: Apr 28 23:10:35 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 23:07:52 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	132154	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	592922	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	383171	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	928367	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1074043	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	810316	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.31	96	12436	4.33	ng/uL	0.00
5) Phenol-d5	6.99	99	311428	21.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	241515	24.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	224895	24.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	237802	21.25	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	120339	24.93	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	134625	26.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.23	165	254157	25.03	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	329362	26.92	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	907006	27.21	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1077899	26.81	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	133893	20.82	ng/ul	0.00
57) Fluorene-d10	15.46	176	813784	27.05	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	106429	16.25	ng/ul	0.00
70) Anthracene-d10	17.32	188	1376630	28.88	ng/ul	0.00
76) Pyrene-d10	19.61	212	1587930	33.50	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1164923	29.56	ng/ul	0.00

Target Compounds						Qvalue
44) Dimethylphthalate	13.92	163	162952	4.94	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM009790.D

Acq On : 28 Apr 2017 21:03

Operator : SJ/MA

Sample : I2845-20

Misc :

ALS Vial : 15 Sample Multiplier: 1

Instrument :

BNA_M

ClientSampleId :

JHT07


Quant Time: Apr 28 23:10:35 2017


Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM042517.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Apr 28 23:07:52 2017

Response via : Initial Calibration

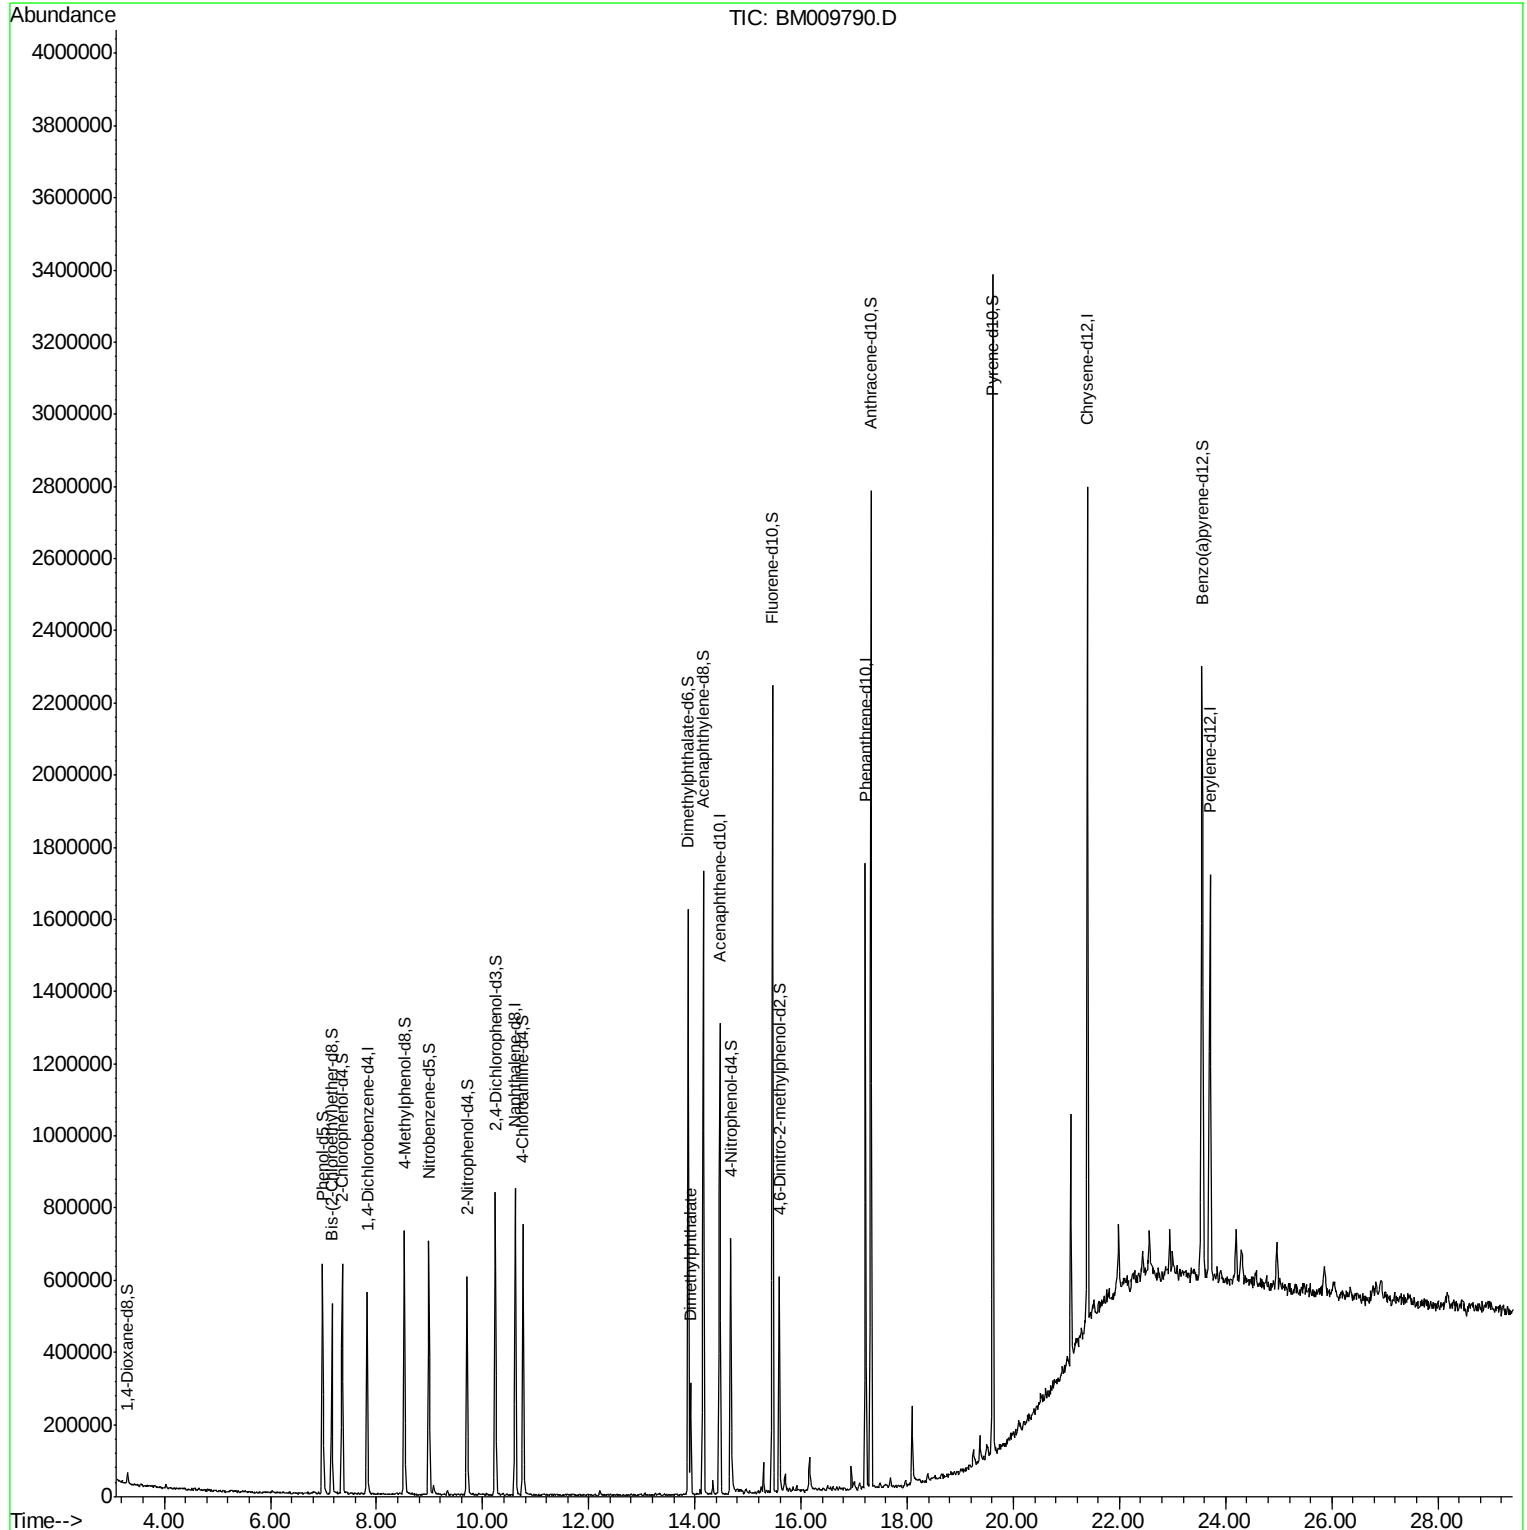

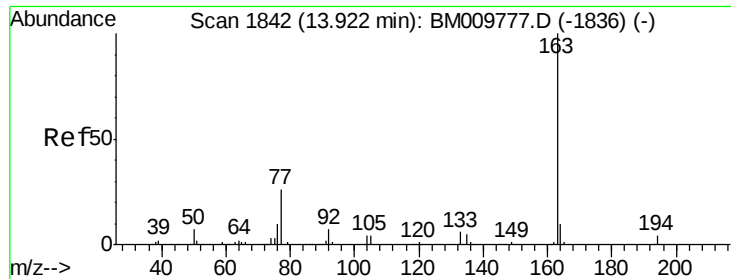

#44

Dimethylphthalate

Concen: 4.94 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BM009790.D

Acq: 28 Apr 2017 21:03

Instrument :

BNA_M

ClientSampleId :

JHT07


Tgt Ion:163 Resp: 162952

Ion Ratio Lower Upper

163 100

194 4.0 3.0 4.6

164 10.2 8.6 12.8

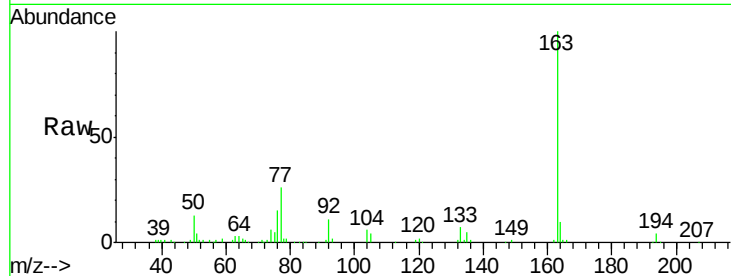

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

