

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042817\
 Data File : BM009782.D
 Acq On : 28 Apr 2017 16:15
 Operator : SJ/MA
 Sample : I2845-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSR1

Quant Time: Apr 28 23:09:18 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 23:07:52 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	100203	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	466267	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.46	164	306436	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	762212	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1035379	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	904473	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	10344	4.75	ng/uL	0.00
5) Phenol-d5	6.98	99	234216	21.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.15	67	172690	23.26	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	158032	22.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	189128	22.29	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	82692	21.79	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	93206	23.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	179513	22.48	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	235754	24.50	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	659520	24.74	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	762282	23.71	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	110828	21.55	ng/ul	0.00
57) Fluorene-d10	15.46	176	589296	24.49	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	93814	17.45	ng/ul	0.00
70) Anthracene-d10	17.32	188	1021654	26.11	ng/ul	0.00
76) Pyrene-d10	19.61	212	1201530	26.30	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1127842	25.64	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.92	163	106387	4.03	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042817\
Data File : BM009782.D
Acq On : 28 Apr 2017 16:15
Operator : SJ/MA
Sample : I2845-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSR1

Quant Time: Apr 28 23:09:18 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 23:07:52 2017
Response via : Initial Calibration

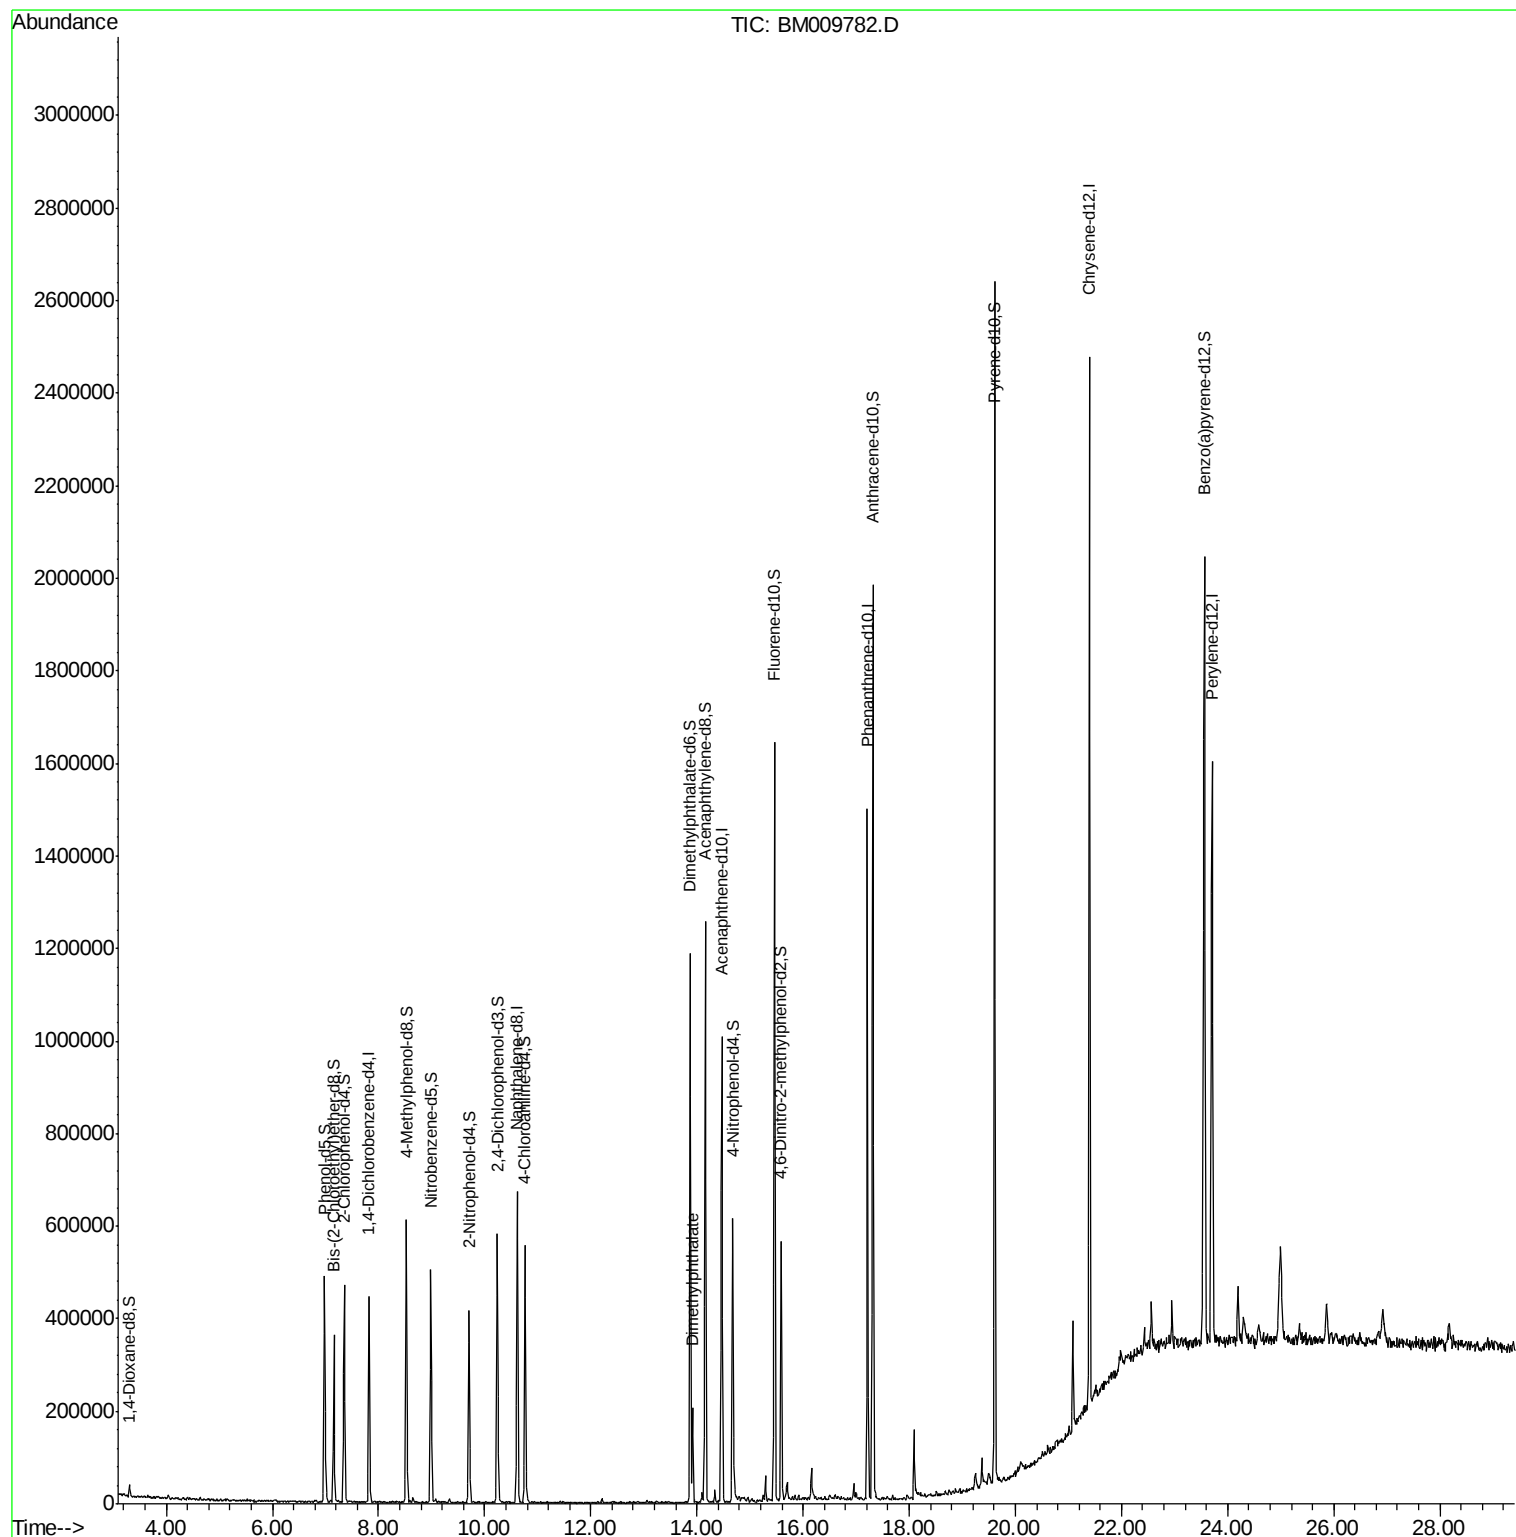

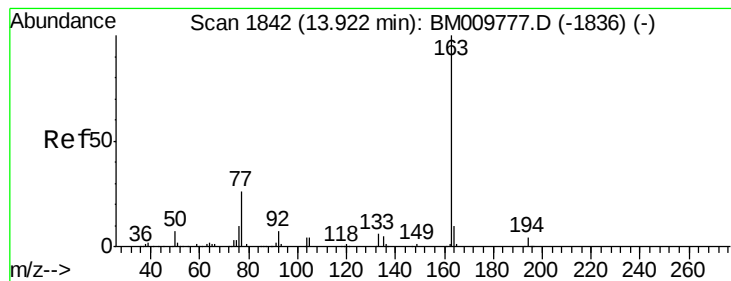

#44

Dimethylphthalate

Concen: 4.03 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BM009782.D

Acq: 28 Apr 2017 16:15

Instrument :

BNA_M

ClientSampleId :

JHSR1


Tot Ion:163 Resp: 106387

Ion Ratio Lower Upper

163 100

194 3.8 3.0 4.6

164 9.9 8.6 12.8

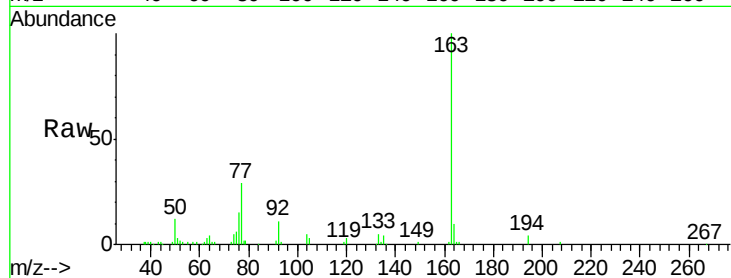

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

