

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042817\
 Data File : BM009785.D
 Acq On : 28 Apr 2017 18:03
 Operator : SJ/MA
 Sample : I2845-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSR4

Quant Time: Apr 28 23:50:47 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Apr 28 23:07:52 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	125435	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	572442	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	376893	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	899543	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	1049500	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	850550	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	25829	9.48	ng/uL	0.00
5) Phenol-d5	6.99	99	538932	39.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	390530	42.03	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	377434	43.54	ng/ul	0.00
13) 4-Methylphenol-d8	8.52	113	452407	42.59	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	203170	43.60	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	229658	46.85	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	431134	43.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	568611	48.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	1447537	44.15	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1783133	45.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.67	143	264850	41.87	ng/ul	0.00
57) Fluorene-d10	15.46	176	1305388	44.11	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	227538	35.85	ng/ul	0.00
70) Anthracene-d10	17.32	188	2152338	46.60	ng/ul	0.00
76) Pyrene-d10	19.62	212	2437308	52.62	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1927784	46.60	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.92	163	199952	6.16	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042817\
Data File : BM009785.D
Acq On : 28 Apr 2017 18:03
Operator : SJ/MA
Sample : I2845-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSR4

Quant Time: Apr 28 23:50:47 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Apr 28 23:07:52 2017
Response via : Initial Calibration

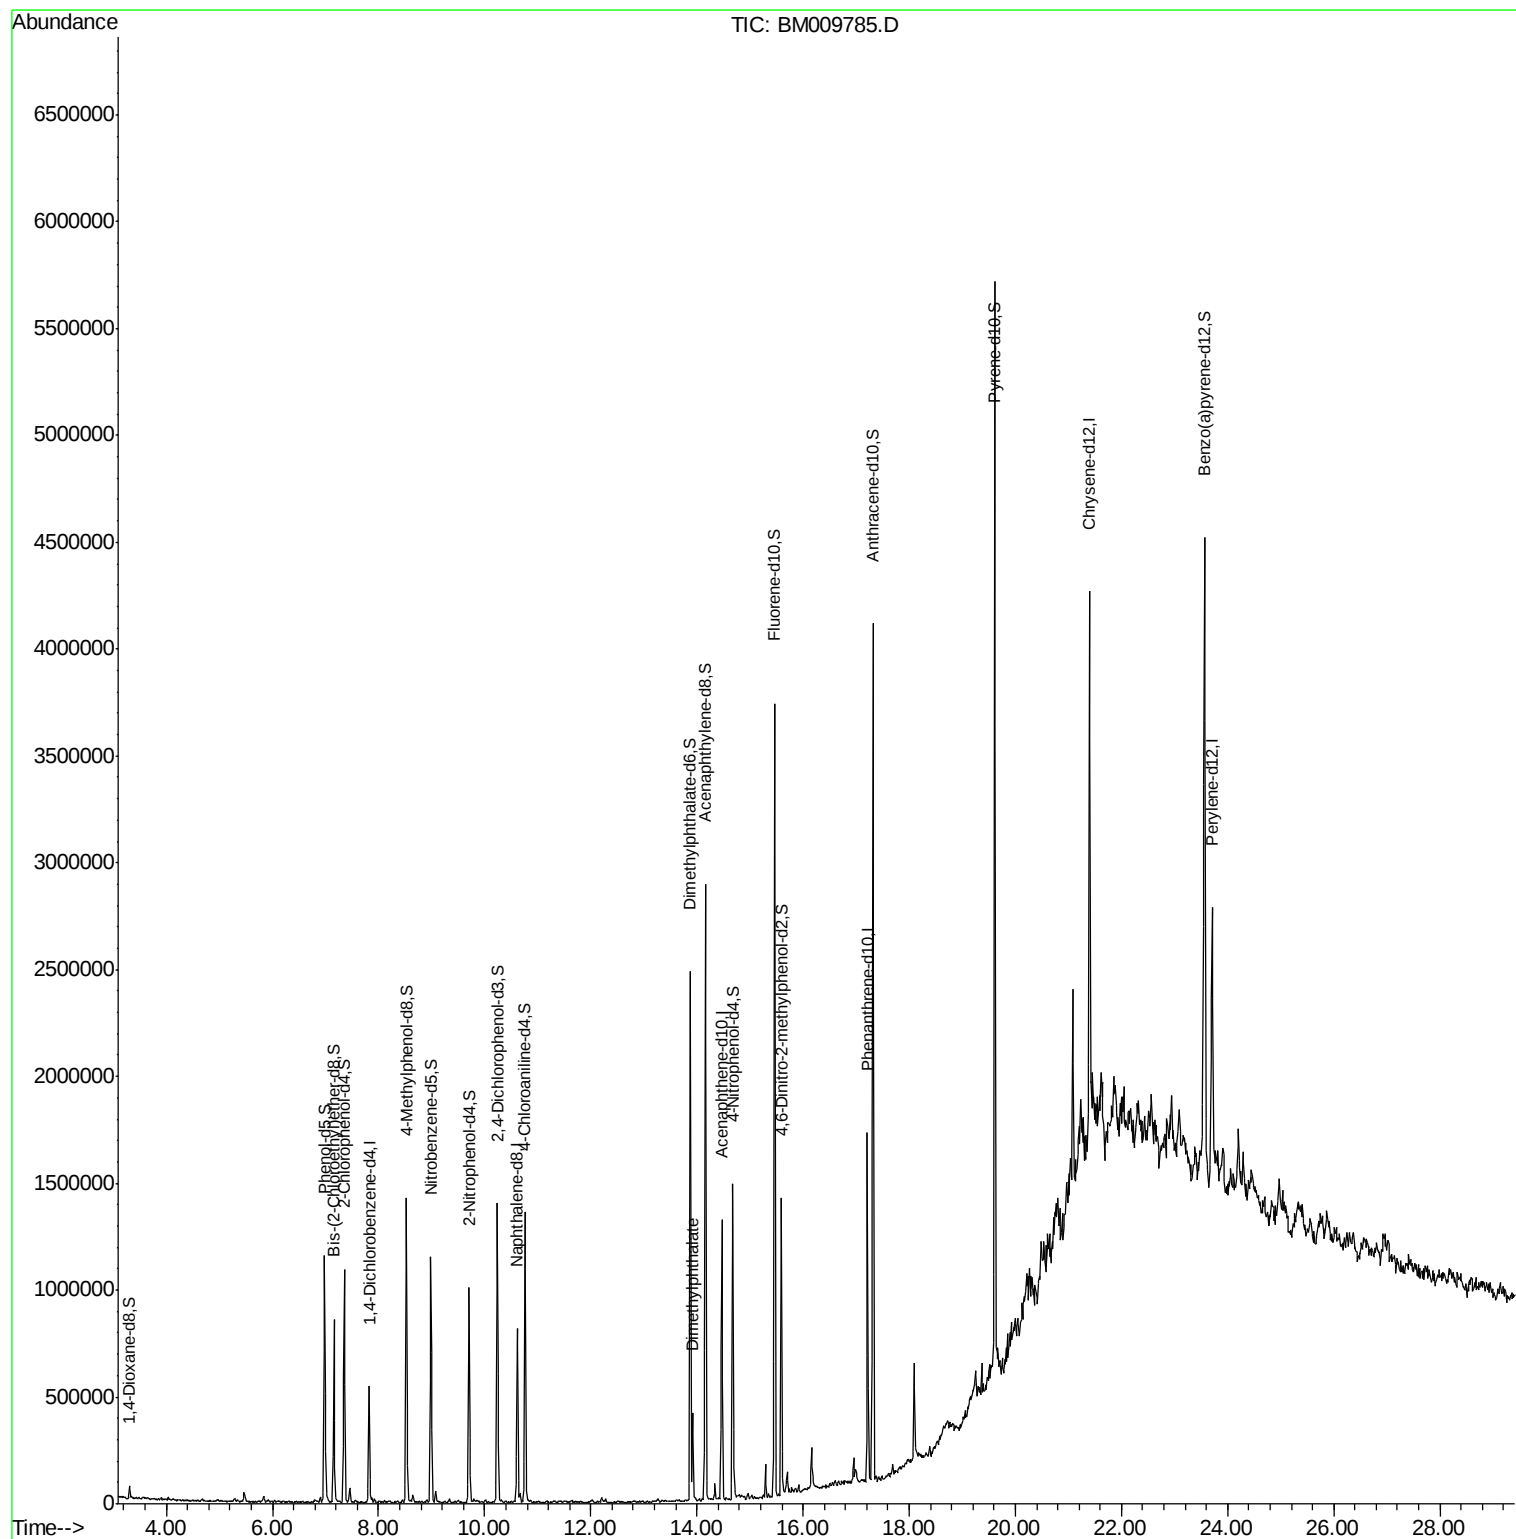

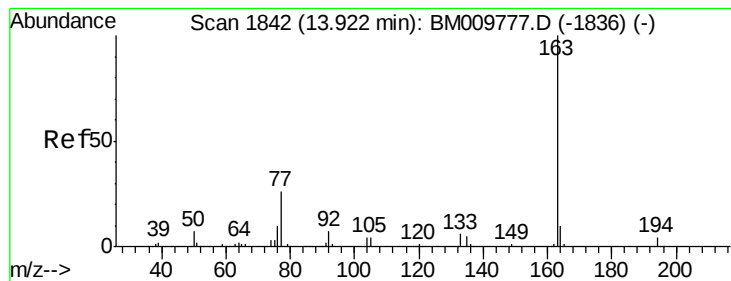

#44

Dimethylphthalate

Concen: 6.16 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BM009785.D

Acq: 28 Apr 2017 18:03

Instrument :

BNA_M

ClientSampleId :

JHSR4


Tot Ion:163 Resp: 199952

Ion Ratio Lower Upper

163 100

194 4.7 3.0 4.6#

164 9.4 8.6 12.8

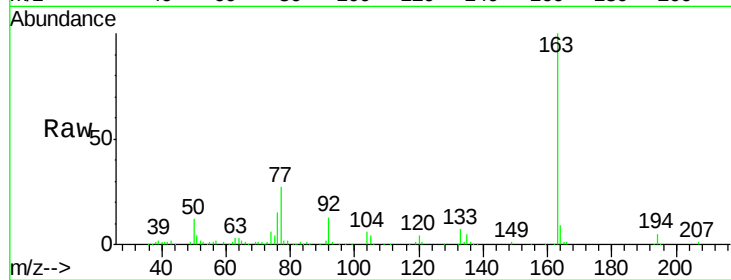

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

