

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042817\
 Data File : BM009797.D
 Acq On : 29 Apr 2017 01:15
 Operator : SJ/MA
 Sample : I2845-18
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JHSX6

Quant Time: Apr 29 03:19:37 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Apr 29 00:28:27 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.82	152	185837	20.00	ng/ul	0.00
18) Naphthalene-d8	10.62	136	784642	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.47	164	480869	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.22	188	1046467	20.00	ng/ul	0.00
75) Chrysene-d12	21.40	240	840654	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	760567	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.30	96	21860	5.42	ng/uL	0.00
5) Phenol-d5	6.99	99	607424	30.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.16	67	398922	28.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.35	132	414073	32.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.53	113	479541	30.47	ng/ul	0.00
19) Nitrobenzene-d5	8.99	128	202578	31.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.70	143	231884	34.51	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.24	165	444068	33.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.76	131	495340	30.59	ng/ul	0.00
43) Dimethylphthalate-d6	13.87	166	1342227	32.09	ng/ul	0.00
46) Acenaphthylene-d8	14.16	160	1710014	33.90	ng/ul	0.00
51) 4-Nitrophenol-d4	14.68	143	215058	26.65	ng/ul	0.00
57) Fluorene-d10	15.46	176	1217806	32.25	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.59	200	135483	18.35	ng/ul	0.00
70) Anthracene-d10	17.32	188	1869263	34.79	ng/ul	0.00
76) Pyrene-d10	19.61	212	1777501	47.91	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.56	264	1260383	34.07	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.92	163	230701	5.57	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM042817\
Data File : BM009797.D
Acq On : 29 Apr 2017 01:15
Operator : SJ/MA
Sample : I2845-18
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JHSX6

Quant Time: Apr 29 03:19:37 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM042517.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Apr 29 00:28:27 2017
Response via : Initial Calibration

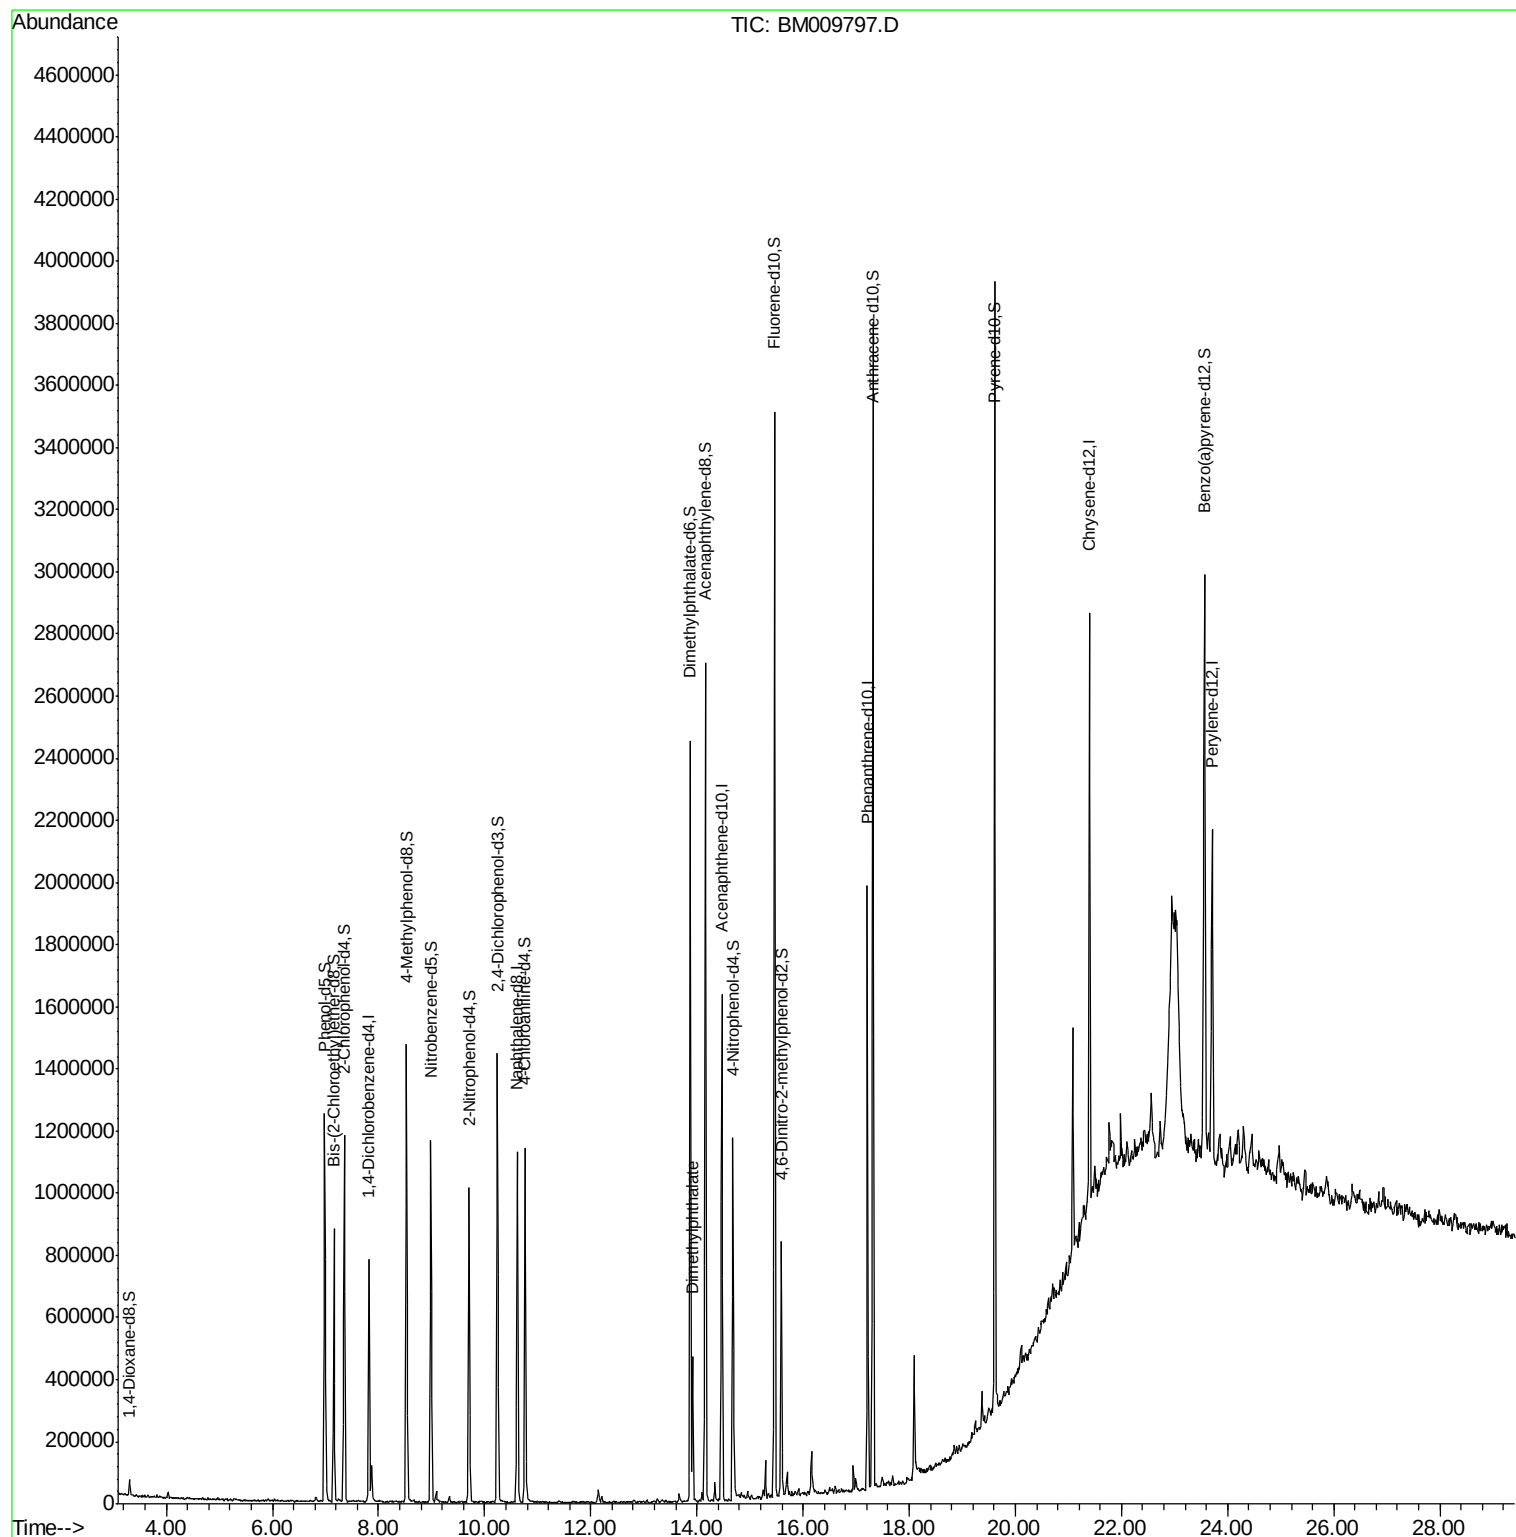

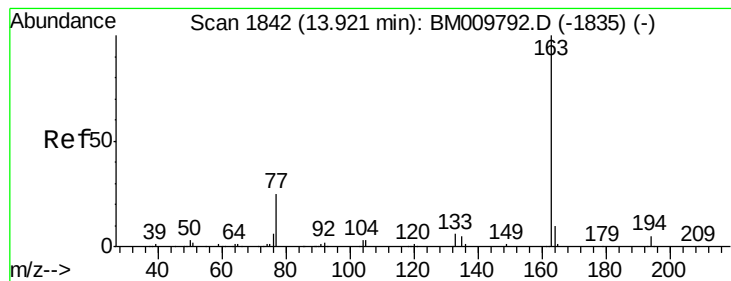

#44

Dimethylphthalate

Concen: 5.57 ng/ul

RT: 13.92 min Scan# 1842

Delta R.T. 0.00 min

Lab File: BM009797.D

Acq: 29 Apr 2017 01:15

Instrument :

BNA_M

ClientSampleId :

JHSX6


Tot Ion:163 Resp: 230701

Ion Ratio Lower Upper

163 100

194 4.0 3.0 4.6

164 11.1 8.6 12.8

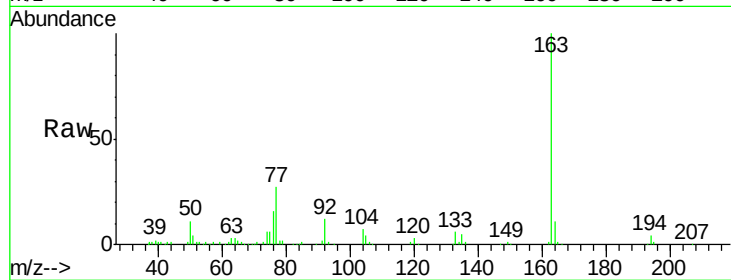

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

