


Data Path : Z:\HPCHEM1\BNA_M\Data\BM042817\
Data File : BM009776.D
Acq On : 28 Apr 2017 12:40
Operator : SJ/MA
Sample : DFTPP08
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP08

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-TEST.M
Title : SVOA CALIBRATION
Last Update : Wed Nov 30 00:32:18 2016

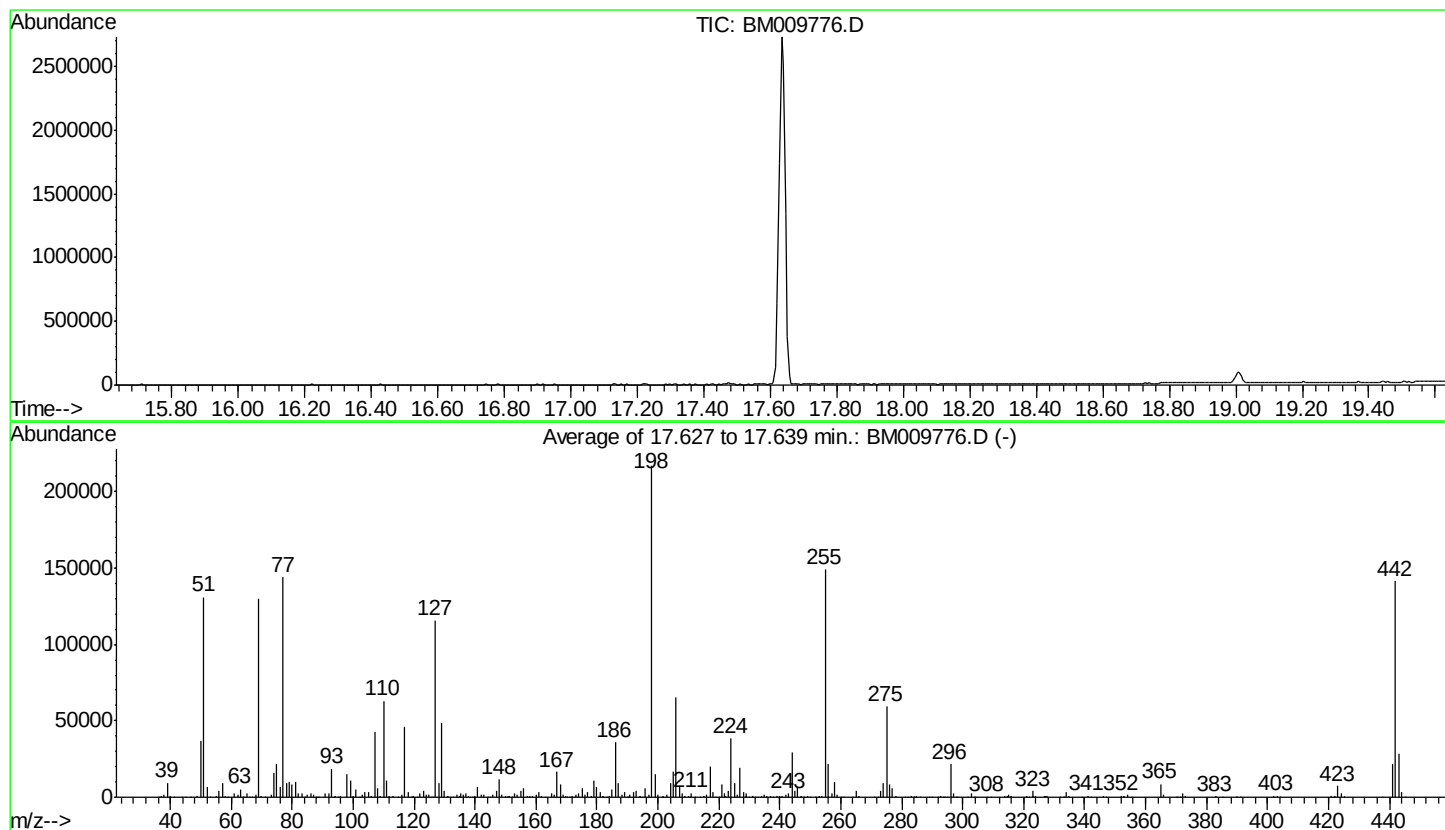

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.2	130672	PASS
68	69	0.00	2	1.6	2102	PASS
69	198	0.00	100	60.0	130117	PASS
70	69	0.00	2	0.6	754	PASS
127	198	10	80	53.2	115469	PASS
197	198	0.00	2	0.6	1302	PASS
198	198	100	100	100.0	216960	PASS
199	198	5	9	7.0	15091	PASS
275	198	10	60	27.3	59200	PASS
365	198	1	100	4.0	8709	PASS
441	443	0.01	100	76.8	22167	PASS
442	198	50	100	65.1	141154	PASS
443	442	15	24	20.5	28874	PASS

m/z	Abundance
36.00	345.0
38.00	929.0
39.00	8104.0
40.00	1145.0
43.90	770.0
49.00	1215.0
50.10	30992.0
51.00	112688.0
52.10	6309.0
53.00	328.0
55.00	768.0
56.00	3722.0
57.00	7674.0
58.10	409.0
59.10	461.0
61.10	2229.0
62.00	1328.0
63.10	4587.0
65.00	2079.0
68.00	1943.0
69.00	106568.0
69.90	992.0
71.00	346.0
73.10	2489.0
74.00	12218.0
75.00	18264.0
76.10	6007.0
77.10	117840.0
78.00	8729.0
79.00	8885.0
80.00	7007.0
81.00	9122.0
82.00	2864.0
83.10	1355.0
85.00	1506.0
86.00	2684.0
87.00	1016.0
87.90	337.0
91.00	2692.0
92.10	2077.0
93.00	14507.0
93.90	1224.0
95.90	908.0
98.00	13342.0
99.00	8871.0
100.00	848.0
101.00	4780.0
102.10	364.0
103.10	1555.0
104.00	3246.0
104.90	3019.0
105.90	837.0
107.00	33152.0
108.00	5317.0
109.00	916.0
110.00	50264.0
111.00	8613.0
112.10	1059.0
116.00	1532.0
117.00	38112.0
117.90	3420.0
118.90	365.0
119.90	376.0
122.00	1817.0
122.90	2984.0
124.00	1308.0
125.00	1151.0
125.90	307.0
127.00	91136.0
128.00	7818.0
129.00	35552.0
130.00	3534.0
130.80	658.0
131.20	470.0
132.10	350.0
133.00	625.0
133.90	1052.0
134.90	2674.0
136.10	1775.0
137.00	2196.0
139.90	492.0
141.00	5551.0
142.10	1668.0
143.00	1015.0
146.10	1692.0
146.90	2827.0
148.00	8005.0
149.00	1865.0
151.10	589.0
151.90	374.0
152.90	1565.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

153.90	1210.0
155.00	2910.0
156.00	3931.0
156.90	1009.0
158.00	797.0
158.80	1099.0
159.90	1365.0
161.00	2042.0
161.90	915.0
165.00	1526.0
165.90	1747.0
167.00	11930.0
168.00	6620.0
169.00	1526.0
170.00	491.0
170.90	863.0
171.90	832.0
172.80	822.0
173.90	1946.0
175.00	3346.0
176.00	2036.0
177.00	1402.0
177.90	1007.0
179.00	7099.0
180.00	5199.0
181.00	2480.0
181.80	642.0
183.90	698.0
184.90	3647.0
186.00	26632.0
187.00	6704.0
188.10	1002.0
188.90	2585.0
189.80	592.0
191.10	998.0
191.90	2879.0
193.00	3749.0
193.90	537.0
196.00	4842.0
197.10	755.0
197.90	161472.0
198.90	11369.0
200.10	920.0
201.60	1122.0
202.90	1303.0
204.00	7121.0
205.00	12323.0
206.00	44520.0
207.10	6683.0
208.00	2189.0
209.00	603.0
210.50	1337.0
211.00	2373.0
214.90	474.0
216.20	835.0
217.00	15215.0
217.90	2504.0
220.20	348.0
221.10	5023.0
221.80	1956.0
222.10	1982.0
223.00	3632.0
224.00	24840.0
225.00	6842.0
225.90	827.0
227.00	13096.0
227.90	2474.0
228.80	2234.0
230.90	1682.0
234.10	702.0
234.90	792.0
235.90	1021.0
236.80	1643.0
237.80	338.0
239.00	458.0
239.80	422.0
240.80	716.0
242.00	1650.0
242.90	1341.0
244.00	21168.0
245.00	3621.0
245.90	4499.0
246.90	1506.0
247.70	303.0
249.00	710.0
250.00	300.0
253.10	725.0
253.90	655.0
255.00	107480.0
256.00	16432.0
256.90	1557.0
258.00	5728.0
259.00	1044.0
265.00	3115.0
273.00	2596.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

273.90	7432.0
275.00	36744.0
276.00	5327.0
277.00	3835.0
277.90	950.0
281.10	418.0
282.90	906.0
285.10	586.0
293.00	518.0
294.00	418.0
296.00	17176.0
296.90	1983.0
302.90	1784.0
303.90	384.0
308.00	491.0
313.90	549.0
314.80	1652.0
316.00	557.0
320.80	335.0
321.90	340.0
322.90	3837.0
324.00	768.0
326.90	869.0
327.70	334.0
334.00	2192.0
334.80	518.0
341.10	517.0
346.00	672.0
352.10	674.0
352.80	673.0
354.00	1016.0
365.00	5596.0
366.00	350.0
372.10	1619.0
373.00	509.0
389.80	333.0
401.80	545.0
403.00	753.0
421.00	728.0
421.80	314.0
422.20	320.0
423.10	3713.0
424.10	1260.0
441.00	12495.0
442.00	78440.0
443.10	16888.0
444.00	2259.0
445.10	316.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

m/z	Abundance
37.00	1233.0
38.00	1859.0
39.10	10616.0
40.00	1744.0
41.00	805.0
44.00	946.0
44.90	351.0
49.10	1165.0
50.00	43736.0
51.00	153344.0
52.00	7370.0
54.90	1110.0
56.00	5399.0
57.00	11703.0
57.90	684.0
58.90	326.0
61.00	2461.0
62.10	2452.0
63.10	6144.0
63.90	937.0
65.00	2662.0
65.90	480.0
66.90	568.0
68.00	2381.0
69.00	157568.0
70.00	816.0
73.00	2816.0
74.00	19600.0
75.00	26496.0
76.00	8946.0
77.10	172352.0
78.10	11985.0
79.10	13044.0
80.00	9476.0
81.00	12496.0
82.00	2936.0
83.00	2791.0
84.00	466.0
85.00	1718.0
86.00	3353.0
86.80	1368.0
88.00	811.0
88.90	499.0
91.00	2634.0
92.00	3028.0
93.00	24264.0
94.10	896.0
96.00	1625.0
98.00	16696.0
99.00	13918.0
100.00	1330.0
100.90	6320.0
102.00	496.0
102.90	1402.0
103.90	4069.0
105.00	4172.0
106.00	1073.0
107.00	50032.0
108.00	7814.0
109.00	1567.0
110.00	78048.0
111.00	13975.0
112.00	1639.0
112.80	1209.0
114.90	320.0
116.00	2619.0
117.00	52376.0
117.90	3293.0
119.80	494.0
121.10	336.0
122.00	4007.0
123.00	5625.0
124.00	2369.0
124.90	1286.0
125.80	422.0
126.20	646.0
127.00	136960.0
128.10	11031.0
129.00	57520.0
130.00	4884.0
131.00	869.0
132.00	383.0
133.10	350.0
134.00	2082.0
135.10	3992.0
135.90	2580.0
137.00	2917.0
137.90	752.0
139.10	626.0
140.00	1056.0
141.00	6757.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

142.00	2120.0
143.00	1828.0
144.00	538.0
145.90	1398.0
147.00	4289.0
148.00	13628.0
149.00	1952.0
150.00	824.0
151.20	819.0
151.90	470.0
152.80	2797.0
154.00	1493.0
155.00	5509.0
156.00	6055.0
157.00	1050.0
158.10	988.0
158.90	1565.0
160.00	2136.0
161.00	4130.0
161.90	1103.0
164.90	3271.0
165.90	1846.0
167.00	19856.0
167.90	10551.0
168.90	1717.0
169.90	562.0
170.30	519.0
170.80	425.0
171.90	1213.0
173.00	3091.0
173.90	2961.0
175.00	6602.0
176.00	1867.0
177.00	3761.0
178.00	1172.0
178.90	14387.0
179.90	9005.0
181.00	4088.0
182.00	858.0
183.00	464.0
184.00	1027.0
185.00	5065.0
186.00	42456.0
187.00	10257.0
188.10	1948.0
189.00	3110.0
190.20	408.0
190.90	1656.0
192.00	3793.0
193.00	4459.0
193.90	1135.0
196.00	7205.0
197.00	1419.0
197.90	253504.0
199.00	16768.0
200.00	1975.0
201.50	1567.0
203.00	1693.0
203.90	11879.0
205.00	19968.0
206.00	76776.0
207.10	11023.0
208.10	3448.0
209.00	1891.0
209.90	1121.0
210.90	3502.0
213.90	314.0
214.90	1515.0
216.00	2085.0
217.00	21792.0
218.00	3705.0
221.10	11898.0
221.90	3630.0
223.00	3615.0
224.00	45032.0
225.00	11839.0
226.00	2030.0
227.00	22704.0
228.00	2783.0
229.00	3479.0
231.10	1448.0
232.10	334.0
232.80	408.0
234.00	1142.0
235.00	2285.0
235.80	941.0
237.10	2048.0
238.90	960.0
239.70	530.0
240.10	808.0
240.80	972.0
242.00	2607.0
242.80	2631.0
244.00	34344.0
245.00	3515.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

246.00	8499.0
246.80	693.0
247.10	822.0
247.90	500.0
248.90	980.0
251.90	330.0
253.20	602.0
253.90	674.0
255.00	168896.0
256.00	25208.0
256.90	2288.0
258.00	13481.0
258.90	1762.0
260.00	902.0
260.90	635.0
265.00	5231.0
266.00	1065.0
270.80	777.0
272.10	451.0
273.00	4675.0
274.00	11035.0
275.00	70976.0
276.00	10306.0
277.00	6270.0
278.00	1266.0
280.90	388.0
282.00	358.0
283.00	1273.0
284.10	625.0
284.90	1268.0
285.90	425.0
290.00	322.0
293.00	1066.0
294.10	314.0
296.00	24672.0
296.90	2791.0
297.90	389.0
302.90	2526.0
304.10	1160.0
309.10	436.0
314.00	838.0
315.00	1883.0
315.90	1843.0
321.00	1032.0
322.00	617.0
323.10	5839.0
324.00	941.0
327.10	1352.0
327.80	501.0
332.00	447.0
333.00	375.0
334.00	4537.0
335.00	1126.0
339.00	326.0
341.10	1120.0
346.00	1512.0
346.80	404.0
352.10	1136.0
353.00	1524.0
354.10	1692.0
355.20	373.0
365.00	9493.0
365.90	1621.0
370.10	334.0
372.10	3228.0
373.00	1014.0
383.00	578.0
390.00	553.0
402.00	1320.0
403.10	1023.0
404.00	457.0
421.00	994.0
422.00	998.0
423.00	8894.0
424.10	3390.0
424.90	417.0
441.10	25640.0
442.10	150656.0
443.10	33152.0
444.10	3783.0
445.10	382.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

m/z	Abundance
37.10	586.0
38.10	1635.0
39.10	10051.0
40.00	1271.0
41.20	301.0
44.00	507.0
46.90	333.0
48.90	1451.0
50.00	36848.0
51.00	125984.0
52.00	6655.0
54.90	509.0
56.00	4206.0
57.00	7241.0
58.10	622.0
61.00	1970.0
62.00	1437.0
63.00	5037.0
64.10	641.0
65.10	2441.0
68.00	1983.0
69.00	126216.0
70.00	456.0
73.00	2357.0
74.00	14815.0
75.00	19792.0
76.00	6201.0
77.10	141760.0
78.00	8268.0
79.00	7609.0
80.00	8790.0
81.00	8263.0
81.90	2818.0
83.00	2321.0
84.10	623.0
85.00	2162.0
86.00	2309.0
86.90	1543.0
88.30	435.0
91.10	1677.0
92.00	3191.0
93.00	16712.0
94.00	857.0
94.90	412.0
96.00	1121.0
98.00	14373.0
99.00	10420.0
100.00	870.0
100.90	4919.0
103.00	1850.0
104.00	4037.0
104.90	3180.0
105.90	1670.0
107.00	43936.0
108.00	5239.0
109.10	1235.0
110.00	61264.0
111.00	9863.0
111.90	953.0
112.90	534.0
116.00	1869.0
117.00	47984.0
118.00	2836.0
119.20	651.0
119.90	875.0
122.00	2681.0
122.90	4412.0
124.00	1238.0
124.90	1779.0
127.00	118312.0
128.00	8508.0
129.00	52824.0
129.90	3634.0
131.00	778.0
132.90	447.0
133.90	1521.0
135.10	3960.0
135.90	1156.0
137.00	1906.0
137.70	615.0
138.10	439.0
139.00	406.0
139.90	1492.0
140.90	7216.0
142.00	2499.0
143.00	1991.0
145.00	334.0
146.00	1325.0
146.90	4388.0
148.00	12514.0
148.90	1634.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

150.10	599.0
150.90	1389.0
153.00	2739.0
154.00	1884.0
155.10	3653.0
156.00	6874.0
157.10	850.0
158.00	1174.0
159.00	935.0
160.00	2618.0
161.10	3454.0
162.00	1155.0
162.90	443.0
165.00	3108.0
165.90	2327.0
167.00	17544.0
168.00	8605.0
169.00	1067.0
169.80	521.0
171.90	1390.0
173.00	1909.0
174.00	3448.0
175.00	7134.0
176.00	1720.0
177.00	3902.0
178.10	1184.0
178.90	11185.0
179.90	6404.0
181.00	3890.0
181.90	950.0
183.80	538.0
185.00	5649.0
186.00	38224.0
187.00	11998.0
188.00	1205.0
189.00	4106.0
189.80	462.0
190.90	1270.0
192.00	3440.0
193.00	4620.0
194.10	690.0
194.80	414.0
195.90	6410.0
196.90	1734.0
197.90	235904.0
198.90	17136.0
200.10	1516.0
201.80	886.0
202.90	2185.0
204.10	9718.0
205.00	18456.0
206.00	74256.0
207.00	9352.0
208.00	2869.0
209.00	849.0
210.00	1766.0
211.00	2702.0
212.10	767.0
214.90	1545.0
216.00	2397.0
217.00	22896.0
217.90	3775.0
219.00	541.0
220.10	413.0
221.10	8796.0
221.90	2144.0
223.00	5410.0
224.00	45136.0
225.00	8982.0
226.00	1495.0
226.90	23072.0
228.00	3842.0
229.00	4297.0
229.90	614.0
231.00	1948.0
234.00	1593.0
235.00	1404.0
235.90	1191.0
236.90	1973.0
238.90	696.0
240.00	1073.0
240.80	1314.0
241.90	2098.0
243.00	2942.0
244.00	33536.0
245.00	5031.0
246.00	6824.0
247.00	1270.0
248.00	314.0
249.00	2023.0
251.70	432.0
253.00	989.0
254.00	1014.0
255.00	169728.0
256.00	24976.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

257.00	2613.0
258.00	11027.0
259.00	1932.0
260.10	301.0
263.90	559.0
265.00	4738.0
266.00	668.0
273.00	6178.0
274.00	10220.0
275.00	69880.0
276.00	8343.0
277.00	7230.0
277.90	1313.0
280.90	840.0
281.80	427.0
283.00	974.0
283.80	519.0
285.00	1407.0
289.00	680.0
292.00	384.0
292.90	1704.0
293.80	791.0
295.00	581.0
296.00	23048.0
297.00	3431.0
298.10	475.0
301.80	476.0
303.00	2321.0
303.90	592.0
308.10	536.0
314.00	1303.0
315.00	2950.0
316.10	1490.0
321.00	931.0
323.00	6334.0
324.00	1213.0
326.80	1952.0
327.90	870.0
332.10	556.0
333.20	622.0
334.00	3772.0
335.00	1081.0
339.00	371.0
341.00	1014.0
342.10	321.0
346.00	999.0
352.10	2052.0
353.00	1110.0
354.10	1807.0
355.20	403.0
365.00	11040.0
365.90	2202.0
370.70	448.0
371.20	330.0
372.10	3681.0
373.10	768.0
383.00	1387.0
385.10	411.0
391.10	331.0
401.90	1438.0
403.10	1939.0
403.90	780.0
421.00	1671.0
422.00	1249.0
423.00	9799.0
424.00	1980.0
425.10	445.0
437.70	321.0
441.00	28368.0
442.10	194368.0
443.00	36584.0
444.10	3802.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08

Scan 2467 (17.598 min): BM009776.D
DFTPP08

m/z	Abundance
39.90	761.0
41.00	356.0
42.90	345.0
44.00	586.0
73.10	1025.0
83.90	340.0
95.90	361.0
132.90	327.0
193.10	390.0
207.10	1526.0
280.80	443.0

Instrument :
BNA_M
ClientSampleId :
DFTPP08