

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042821\
 Data File : BM029688.D
 Acq On : 28 Apr 2021 12:10
 Operator : CG/JU
 Sample : PB135845BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK845

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM041221.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.940	6	9	12	rBV	11612	9767	0.72%	0.145%
2	2.969	12	14	16	rVV2	5915	4318	0.32%	0.064%
3	2.993	16	18	20	rVV3	5541	4482	0.33%	0.066%
4	3.028	20	24	29	rVB	596310	626234	46.40%	9.276%
5	3.363	77	81	86	rVB	18249	22454	1.66%	0.333%
6	3.834	157	161	165	rVB	8703	10598	0.79%	0.157%
7	4.769	317	320	326	rVB4	2699	4006	0.30%	0.059%
8	4.863	333	336	340	rBV5	1005	1539	0.11%	0.023%
9	7.416	764	770	774	rBV6	823	1954	0.14%	0.029%
10	7.528	787	789	794	rVB4	960	1368	0.10%	0.020%
11	7.610	794	803	815	rBV	345002	562728	41.69%	8.335%
12	10.392	1268	1276	1291	rBV	411457	715967	53.05%	10.605%
13	14.263	1927	1934	1951	rBV	654179	1035797	76.75%	15.342%
14	16.792	2361	2364	2368	rVV3	2079	2938	0.22%	0.044%
15	16.827	2368	2370	2374	rVB3	1012	1499	0.11%	0.022%
16	17.004	2394	2400	2414	rBV	815263	1240969	91.95%	18.381%
17	17.915	2549	2555	2560	rBV7	4065	7621	0.56%	0.113%
18	18.586	2667	2669	2672	rBV3	1248	1400	0.10%	0.021%
19	18.668	2681	2683	2685	rBV2	1360	1360	0.10%	0.020%
20	21.186	3106	3111	3122	rBV	968644	1349647	100.00%	19.991%
21	23.374	3477	3483	3495	rVB2	597749	1144711	84.82%	16.955%


Sum of corrected areas: 6751357

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042821\
Data File : BM029688.D
Acq On : 28 Apr 2021 12:10
Operator : CG/JU
Sample : PB135845BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK845

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM041221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

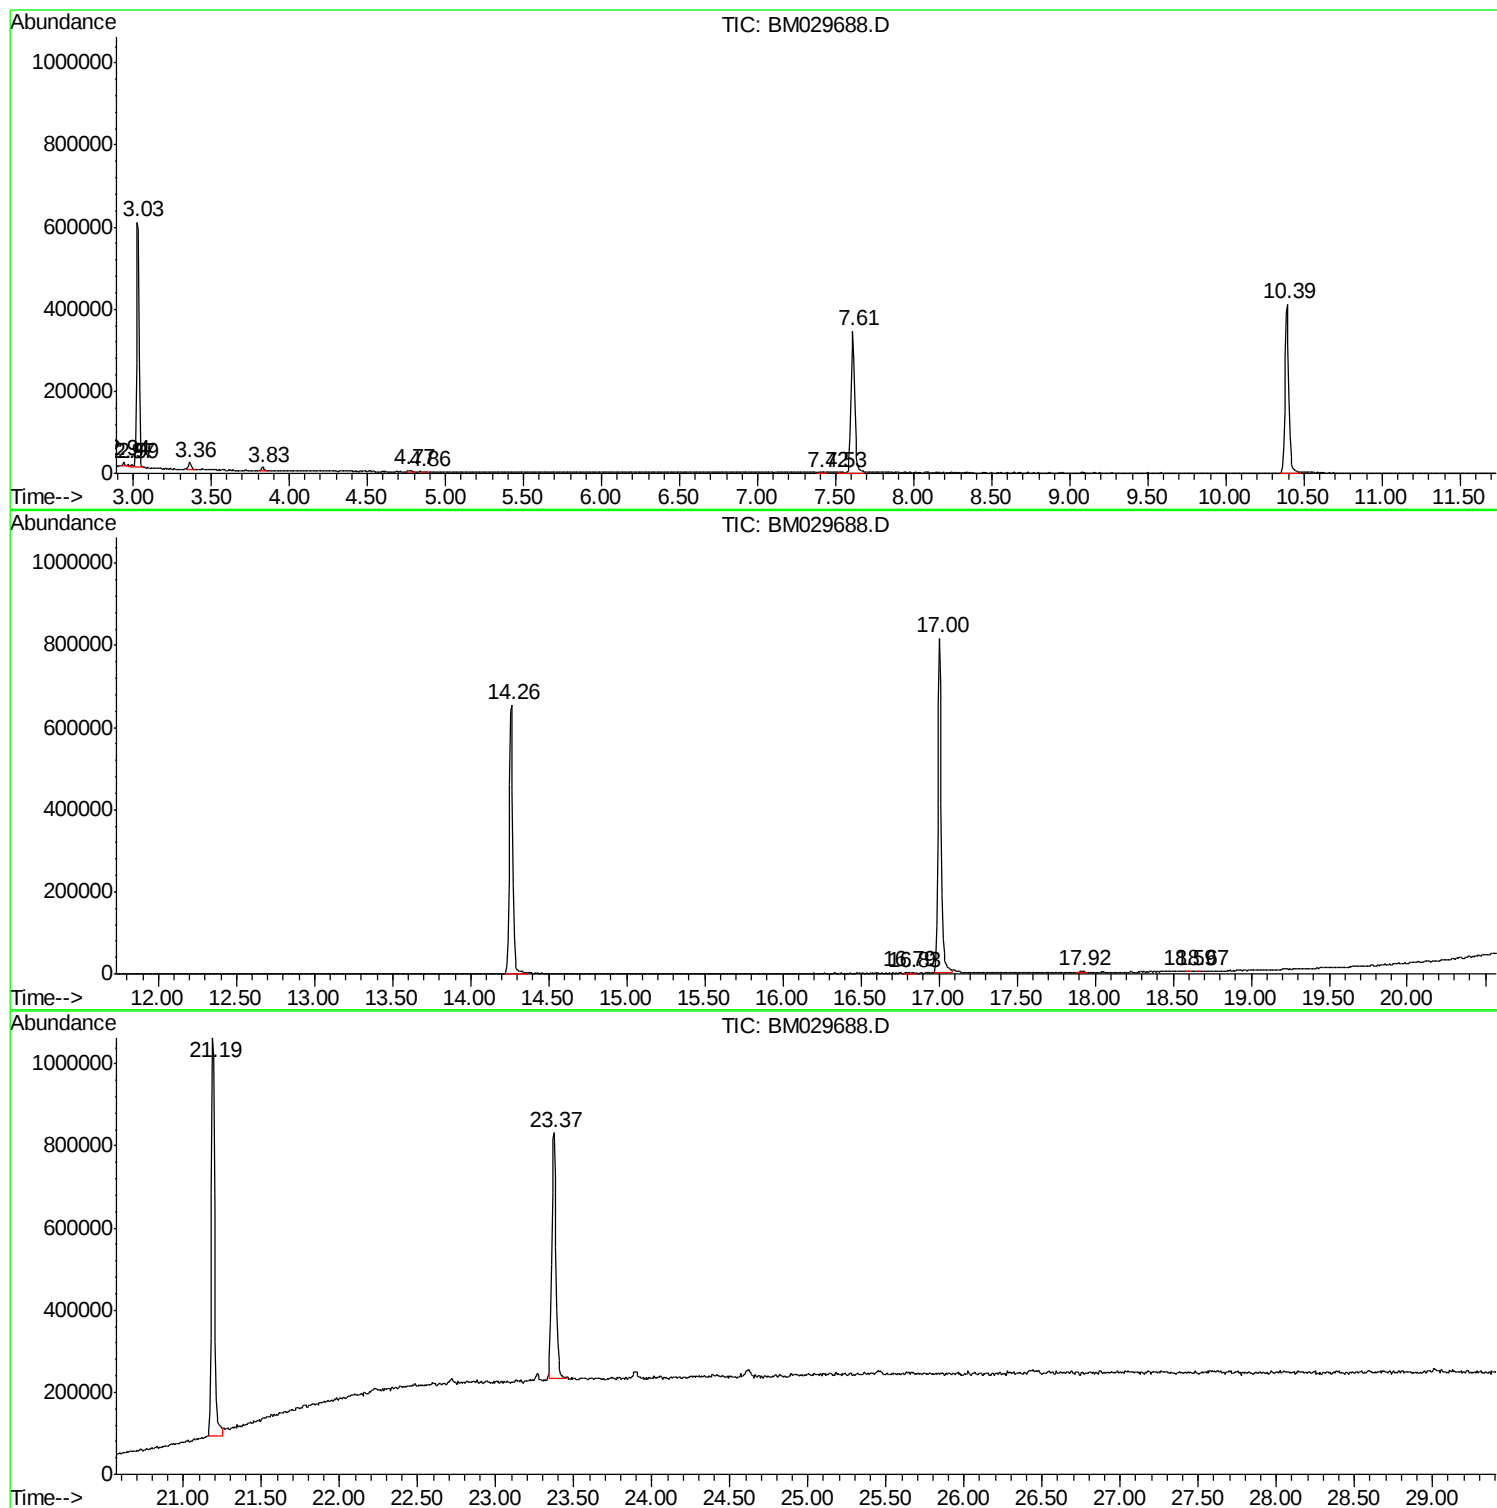

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM042821\
Data File : BM029688.D
Acq On : 28 Apr 2021 12:10
Operator : CG/JU
Sample : PB135845BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK845










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM041221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.03	22.26 ng/ul	626234	1,4-Dichlorobenzene-d4	7.61

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptane	100	C7H16	000142-82-5	91
2		Heptane	100	C7H16	000142-82-5	91
3		Heptane	100	C7H16	000142-82-5	90
4		Heptane	100	C7H16	000142-82-5	87
5		Butane, 2,2-dimethyl-	86	C6H14	000075-83-2	43

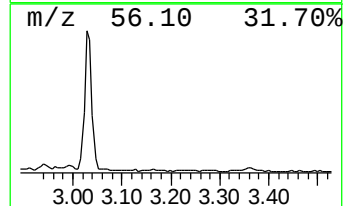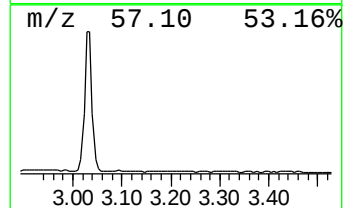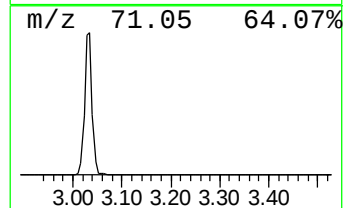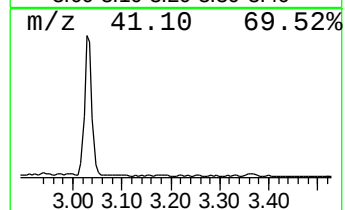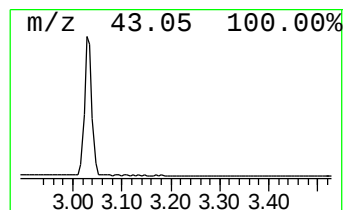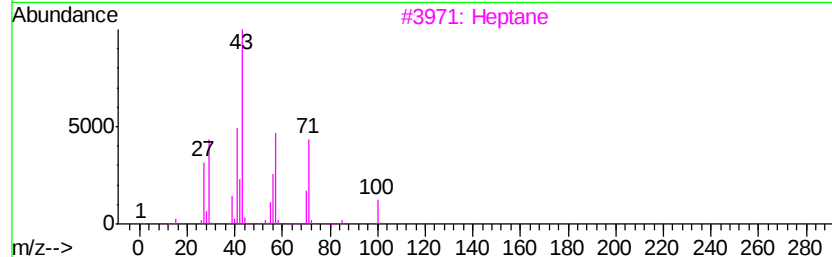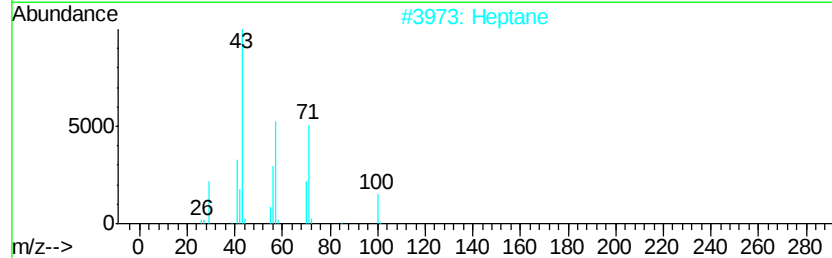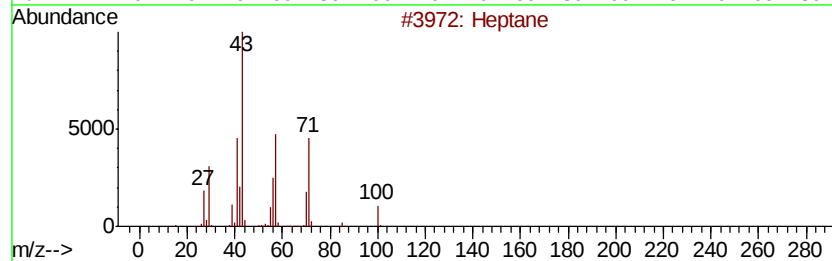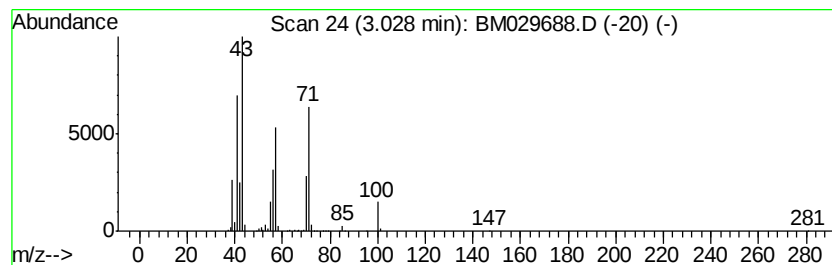

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM042821\
Data File : BM029688.D
Acq On : 28 Apr 2021 12:10
Operator : CG/JU
Sample : PB135845BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK845

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM041221.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	3.03	22.3	ng/ul	626234	1	7.61	562728	20.0