


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM042821\
 Data File : BM029685.D
 Acq On : 28 Apr 2021 10:02
 Operator : CG/JU
 Sample : DFTPP001
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP001

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM041221.M
 Title : SVOA CALIBRATION
 Last Update : Wed Apr 28 12:12:26 2021

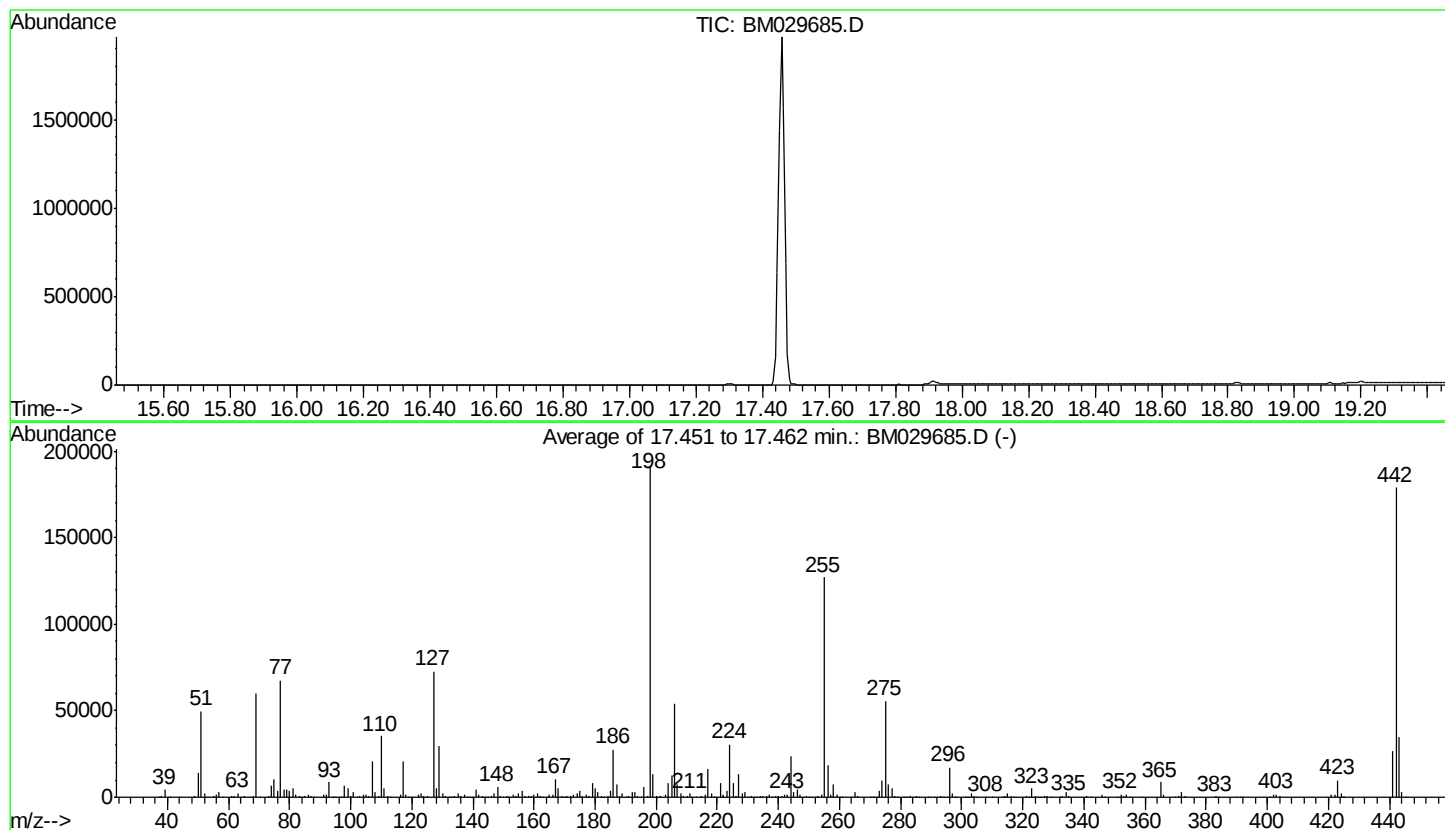

AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.1	49962	PASS
68	69	0.00	2	1.5	884	PASS
69	198	0.00	100	31.4	60248	PASS
70	69	0.00	2	0.5	300	PASS
127	198	10	80	37.9	72669	PASS
197	198	0.00	2	0.6	1086	PASS
198	198	100	100	100.0	191701	PASS
199	198	5	9	6.8	13076	PASS
275	198	10	60	29.1	55797	PASS
365	198	1	100	4.5	8625	PASS
441	198	0.01	100	13.9	26613	PASS
442	198	50	100	93.4	178989	PASS
443	442	15	24	19.3	34474	PASS

Scan 2470 (17.415 min): BM029685.D
DFTPP001

m/z	Abundance
39.90	164.0
44.00	424.0
73.00	239.0
192.90	214.0
207.00	810.0
207.90	268.0
281.10	295.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

m/z	Abundance
36.90	316.0
38.00	719.0
39.00	4089.0
40.00	437.0
41.00	214.0
44.00	585.0
49.10	613.0
50.10	14520.0
51.10	52048.0
52.10	2568.0
55.00	457.0
56.10	1430.0
57.00	3110.0
61.00	590.0
62.00	854.0
63.00	2222.0
63.90	319.0
65.10	1005.0
67.00	161.0
69.00	60232.0
70.00	238.0
73.00	1011.0
74.00	6164.0
75.00	9719.0
76.10	3653.0
77.10	68384.0
78.10	4792.0
79.00	5154.0
80.00	3558.0
81.00	5063.0
82.00	1046.0
83.00	1259.0
85.00	891.0
86.00	1567.0
87.00	658.0
87.90	317.0
91.00	1219.0
92.10	1516.0
93.00	8642.0
93.90	544.0
95.00	183.0
96.00	432.0
97.10	198.0
98.00	6762.0
99.00	5677.0
100.00	488.0
101.00	2973.0
102.00	201.0
103.00	850.0
103.90	1790.0
105.00	1463.0
105.90	543.0
107.00	19824.0
108.00	3156.0
109.00	569.0
110.00	34272.0
111.00	5680.0
111.90	731.0
112.90	219.0
116.10	1048.0
117.00	20328.0
118.00	1368.0
119.00	184.0
119.90	362.0
122.00	1449.0
123.00	2286.0
123.90	977.0
124.90	1018.0
127.00	69056.0
128.00	4887.0
129.00	28632.0
130.00	2300.0
131.00	498.0
132.00	257.0
133.10	164.0
134.00	727.0
135.00	2255.0
136.00	1067.0
137.10	1033.0
138.00	361.0
139.90	379.0
141.00	3853.0
142.10	1195.0
142.90	750.0
144.00	294.0
145.00	361.0
146.00	759.0
147.00	1981.0
148.00	5754.0
149.00	1240.0
150.00	332.0
151.10	476.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

151.60	451.0
153.00	1350.0
154.00	906.0
155.00	2155.0
156.00	3691.0
157.00	472.0
158.00	690.0
158.90	553.0
160.00	1267.0
161.00	1959.0
161.90	612.0
163.00	264.0
164.00	238.0
165.00	1414.0
166.10	1445.0
167.00	9891.0
168.00	4800.0
169.00	855.0
169.90	365.0
170.90	418.0
171.90	944.0
173.00	1082.0
174.00	2245.0
175.00	3106.0
176.00	1016.0
177.00	1891.0
178.00	605.0
179.00	7495.0
180.00	4611.0
181.00	2133.0
182.00	375.0
182.90	270.0
184.00	652.0
185.00	3681.0
186.10	24264.0
187.00	7058.0
188.00	1022.0
189.00	1880.0
190.00	356.0
191.00	796.0
192.00	2233.0
193.00	2527.0
194.00	401.0
195.00	489.0
196.00	4835.0
197.10	1576.0
198.00	167680.0
199.00	12101.0
200.00	1037.0
200.80	157.0
201.50	618.0
203.00	1441.0
204.10	6960.0
205.10	11221.0
206.10	47752.0
207.00	6835.0
208.00	1951.0
208.90	755.0
210.10	755.0
211.10	1767.0
211.60	484.0
213.10	154.0
214.90	698.0
216.10	1157.0
217.00	13713.0
218.00	1858.0
218.80	222.0
220.10	182.0
221.00	6897.0
221.70	1616.0
222.00	1450.0
223.00	3353.0
224.00	26176.0
225.00	6575.0
226.00	914.0
227.00	11605.0
228.00	1569.0
229.00	2339.0
229.90	301.0
231.10	818.0
232.10	206.0
234.00	761.0
235.00	955.0
235.90	446.0
237.00	872.0
239.00	484.0
239.90	431.0
241.10	845.0
242.00	1480.0
243.00	1664.0
244.10	20320.0
245.00	2586.0
246.00	3831.0
247.00	1136.0
248.00	243.0
249.00	931.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

250.00	227.0
251.00	214.0
252.00	192.0
253.00	360.0
254.20	892.0
255.00	104688.0
256.00	15672.0
257.00	1218.0
258.00	6538.0
259.00	1255.0
259.90	172.0
260.90	190.0
265.00	2454.0
266.00	423.0
269.90	167.0
272.10	214.0
273.00	3470.0
274.00	8096.0
275.00	44968.0
276.00	5938.0
277.00	3426.0
278.00	605.0
281.00	373.0
282.00	257.0
283.00	433.0
283.90	198.0
285.10	562.0
285.90	166.0
292.10	195.0
293.00	965.0
294.00	238.0
295.10	291.0
296.00	13628.0
297.00	1843.0
298.10	155.0
301.10	187.0
302.10	233.0
303.00	1305.0
304.10	400.0
307.90	195.0
313.00	188.0
314.10	676.0
315.00	1314.0
316.00	890.0
321.10	385.0
322.00	195.0
323.00	3947.0
324.10	836.0
325.10	182.0
327.00	775.0
328.00	552.0
332.00	214.0
333.00	531.0
334.00	2784.0
335.10	642.0
341.00	508.0
342.00	164.0
346.00	1118.0
346.80	189.0
352.00	1299.0
353.10	810.0
354.00	1303.0
355.00	247.0
365.00	6410.0
365.90	1054.0
370.90	378.0
372.00	2073.0
373.00	379.0
383.00	688.0
383.90	159.0
389.90	301.0
391.00	220.0
402.00	875.0
403.00	1179.0
404.10	421.0
421.00	906.0
422.00	1152.0
423.10	6659.0
424.10	1909.0
424.90	363.0
441.10	16976.0
442.10	122184.0
443.10	24160.0
444.10	2382.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

m/z	Abundance
37.00	406.0
38.00	940.0
39.10	4989.0
40.00	369.0
41.00	169.0
44.10	507.0
48.90	630.0
50.10	16832.0
51.10	58488.0
52.10	2915.0
53.00	234.0
55.00	478.0
56.00	1772.0
57.00	3894.0
58.00	251.0
61.00	943.0
62.00	1145.0
63.10	2682.0
64.00	572.0
65.00	1452.0
67.00	255.0
68.10	1610.0
69.00	70760.0
70.10	397.0
73.10	901.0
74.10	7926.0
75.00	12241.0
76.10	4056.0
77.10	79184.0
78.10	5346.0
79.00	4989.0
80.00	4412.0
81.00	5955.0
82.00	1612.0
83.00	1001.0
84.00	217.0
84.90	721.0
86.00	1989.0
87.00	608.0
87.90	367.0
91.00	1424.0
92.00	1514.0
93.00	10142.0
94.10	678.0
95.00	209.0
96.00	446.0
97.00	206.0
98.00	7989.0
99.00	5660.0
100.00	617.0
101.00	2982.0
102.00	254.0
103.00	1316.0
104.00	2255.0
105.00	2376.0
106.00	649.0
107.00	24016.0
108.00	4054.0
109.00	954.0
110.00	41968.0
111.00	6242.0
112.00	783.0
112.90	249.0
116.10	1498.0
117.00	24008.0
118.00	1762.0
118.90	206.0
120.00	245.0
122.00	1816.0
123.00	2914.0
124.00	1347.0
125.00	1072.0
127.00	86016.0
128.00	6625.0
129.00	35032.0
130.00	2894.0
130.90	481.0
132.00	235.0
132.70	164.0
134.00	1224.0
135.00	3014.0
136.00	1057.0
137.10	1650.0
138.00	265.0
138.80	209.0
140.00	374.0
141.00	4848.0
142.00	1403.0
143.00	724.0
144.00	391.0
144.90	238.0
146.00	1089.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

147.00	2657.0
148.00	7164.0
149.00	1227.0
150.00	441.0
151.00	624.0
152.00	507.0
153.00	1761.0
154.00	1384.0
155.00	3119.0
156.00	4186.0
157.00	935.0
158.00	1127.0
159.00	742.0
160.00	2019.0
161.00	2363.0
162.00	565.0
163.00	300.0
164.00	219.0
165.00	2207.0
166.00	1855.0
167.00	12921.0
168.00	6153.0
169.00	1018.0
170.00	291.0
171.00	488.0
172.00	1108.0
173.00	1544.0
174.00	2068.0
175.00	4381.0
176.00	1263.0
177.00	2092.0
178.10	688.0
179.00	9315.0
180.00	6193.0
181.00	3229.0
182.00	483.0
184.00	761.0
185.10	4384.0
186.00	32480.0
187.00	8767.0
188.00	1030.0
189.00	2146.0
190.00	536.0
191.10	1032.0
192.00	3381.0
193.00	3556.0
194.00	700.0
195.10	317.0
196.00	6675.0
197.10	1684.0
198.00	228608.0
199.00	15375.0
200.00	1208.0
200.80	382.0
201.50	1089.0
203.00	1734.0
204.00	9508.0
205.10	15574.0
206.10	63864.0
207.10	9712.0
208.00	2702.0
209.00	1023.0
210.10	905.0
211.00	2633.0
212.90	166.0
215.00	920.0
216.10	1789.0
217.00	19264.0
218.00	2511.0
219.00	224.0
219.90	326.0
221.00	9792.0
221.70	2104.0
223.00	3775.0
224.10	37056.0
225.10	9431.0
226.00	1087.0
227.00	16304.0
228.00	2404.0
229.00	3208.0
230.00	537.0
231.00	1451.0
231.90	213.0
233.00	399.0
234.00	1259.0
235.00	1198.0
236.00	904.0
237.00	1500.0
237.90	187.0
238.90	527.0
239.90	469.0
240.90	834.0
242.00	2077.0
243.00	2058.0
244.10	27976.0
245.00	3926.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

246.00	5595.0
247.00	1378.0
247.90	232.0
249.00	1138.0
249.90	174.0
250.90	349.0
252.00	374.0
253.00	617.0
254.20	1178.0
255.00	152320.0
256.10	22536.0
257.00	1758.0
258.00	8257.0
259.00	1394.0
260.10	292.0
260.90	195.0
264.00	273.0
265.00	4074.0
266.00	784.0
269.90	295.0
271.00	281.0
272.00	442.0
273.00	4826.0
274.00	11069.0
275.00	67896.0
276.00	9414.0
277.00	6331.0
278.00	1113.0
278.90	243.0
281.10	256.0
281.90	291.0
283.10	671.0
283.90	328.0
285.10	1104.0
288.90	191.0
289.90	211.0
292.00	317.0
292.90	1197.0
293.90	344.0
296.00	21272.0
297.00	2919.0
298.00	234.0
301.00	178.0
301.90	339.0
303.10	2253.0
304.00	574.0
305.00	153.0
308.00	331.0
310.00	274.0
313.10	174.0
314.10	963.0
315.00	2576.0
316.00	1030.0
317.00	159.0
321.00	497.0
322.10	360.0
323.10	5910.0
324.00	1114.0
325.00	179.0
325.90	240.0
327.00	1277.0
328.10	668.0
329.00	179.0
332.00	482.0
333.00	724.0
334.10	4055.0
335.00	1016.0
341.10	760.0
346.00	1414.0
346.90	226.0
351.00	169.0
352.00	1752.0
353.00	1188.0
354.10	2195.0
355.10	387.0
358.90	244.0
365.00	10261.0
366.00	1201.0
369.90	222.0
371.00	462.0
372.00	3819.0
373.00	880.0
383.10	646.0
383.90	222.0
389.90	415.0
391.00	374.0
392.00	249.0
400.90	256.0
402.00	1438.0
403.00	2000.0
404.00	803.0
421.00	1546.0
422.00	1375.0
423.00	11066.0
424.10	2986.0
424.90	259.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

441.10	32064.0
442.10	210240.0
443.10	40808.0
444.10	3738.0
445.10	245.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

m/z	Abundance
37.00	207.0
38.00	580.0
39.10	3610.0
39.90	289.0
40.90	162.0
44.00	514.0
49.10	582.0
50.00	10476.0
51.10	39352.0
52.00	1926.0
55.00	265.0
56.00	1219.0
57.00	2646.0
61.00	615.0
62.00	728.0
63.10	2138.0
64.10	216.0
65.00	830.0
67.10	210.0
68.00	1044.0
69.00	49752.0
70.00	267.0
73.00	950.0
74.00	5422.0
75.00	8852.0
76.00	2890.0
77.10	54960.0
78.10	3470.0
79.00	3949.0
80.00	3369.0
81.00	3950.0
82.00	948.0
83.00	867.0
83.90	161.0
85.00	762.0
86.00	1531.0
87.10	477.0
88.00	248.0
91.00	1037.0
92.00	1258.0
93.00	7269.0
94.00	507.0
95.00	156.0
95.90	254.0
96.90	197.0
98.00	5425.0
99.00	3862.0
99.90	407.0
101.00	2147.0
101.90	167.0
103.00	913.0
104.00	1426.0
105.00	1632.0
106.10	566.0
107.00	17584.0
108.00	2655.0
109.10	423.0
110.00	29744.0
111.00	4483.0
112.00	569.0
113.00	287.0
116.10	1113.0
117.00	18600.0
118.00	1330.0
118.90	306.0
120.00	286.0
122.00	1217.0
123.00	2164.0
124.00	822.0
125.00	891.0
127.00	62936.0
128.00	4830.0
129.00	25256.0
130.00	2144.0
131.00	396.0
132.10	245.0
133.00	154.0
133.90	789.0
135.10	2345.0
136.00	1179.0
137.00	1099.0
138.00	275.0
138.90	163.0
140.00	426.0
141.00	4155.0
141.90	1019.0
143.00	806.0
144.00	212.0
144.90	228.0
145.90	706.0
147.00	1892.0
148.00	5649.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

149.00	922.0
150.00	398.0
151.10	456.0
152.00	268.0
153.00	1295.0
154.00	974.0
155.00	1766.0
156.00	2890.0
157.10	571.0
158.00	736.0
159.00	623.0
160.00	1276.0
161.00	1789.0
161.90	617.0
163.00	208.0
164.90	1585.0
166.00	1133.0
167.00	9061.0
168.00	4907.0
169.00	730.0
170.00	370.0
170.90	423.0
172.00	907.0
173.00	1253.0
174.00	1631.0
175.00	3734.0
176.00	888.0
177.00	1619.0
177.90	771.0
179.00	7686.0
180.00	4857.0
181.00	2503.0
182.00	344.0
184.00	690.0
185.00	3794.0
186.00	25560.0
187.10	7332.0
188.00	625.0
189.00	1806.0
189.90	272.0
191.00	921.0
192.00	2548.0
193.00	3086.0
194.00	659.0
195.00	167.0
196.00	5249.0
198.00	178816.0
199.00	11754.0
200.10	965.0
201.30	611.0
203.00	1676.0
204.10	7339.0
205.10	11934.0
206.10	50416.0
207.10	7463.0
208.00	1823.0
209.00	707.0
210.20	741.0
211.10	1754.0
213.00	176.0
215.00	787.0
216.00	1122.0
217.00	15210.0
218.00	1692.0
218.80	163.0
221.10	7366.0
222.10	1727.0
223.00	3117.0
224.00	28760.0
225.10	7979.0
226.00	818.0
227.00	12625.0
228.00	1925.0
229.00	2784.0
230.00	286.0
231.00	1045.0
233.00	168.0
233.90	869.0
235.00	979.0
235.90	665.0
237.00	1135.0
239.00	522.0
240.00	303.0
241.00	816.0
242.00	1568.0
243.10	1758.0
244.10	22376.0
245.00	2845.0
246.00	5000.0
247.00	1256.0
248.00	215.0
249.00	954.0
251.00	345.0
251.90	260.0
252.90	453.0
254.20	1362.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001

255.00	123848.0
256.00	17896.0
257.00	1299.0
258.00	7272.0
259.00	1136.0
260.00	284.0
260.80	153.0
263.80	219.0
265.00	2779.0
266.00	367.0
271.20	239.0
272.00	242.0
273.00	3940.0
274.00	9920.0
275.00	54528.0
276.00	7739.0
277.00	5355.0
278.00	793.0
278.90	197.0
281.10	376.0
283.10	524.0
284.00	520.0
285.10	1052.0
286.00	177.0
288.80	220.0
290.00	170.0
291.00	167.0
292.00	225.0
293.00	984.0
294.00	389.0
295.10	365.0
296.00	17040.0
297.00	2564.0
297.80	174.0
301.00	191.0
301.90	300.0
303.00	2101.0
304.10	554.0
307.90	174.0
310.00	227.0
313.00	163.0
313.90	822.0
315.00	2053.0
316.00	1115.0
317.00	156.0
321.10	548.0
322.00	298.0
323.10	5356.0
324.10	934.0
325.00	167.0
327.00	1036.0
327.90	578.0
332.00	384.0
333.00	490.0
334.00	3162.0
335.00	1091.0
341.00	654.0
341.90	154.0
346.00	1349.0
346.90	162.0
352.00	1722.0
353.00	1200.0
354.00	1497.0
355.10	435.0
365.00	9204.0
366.00	1409.0
370.00	182.0
371.10	551.0
372.10	3267.0
373.10	702.0
383.00	794.0
383.90	277.0
390.00	356.0
390.90	171.0
392.00	201.0
400.90	237.0
402.00	1405.0
403.00	2053.0
404.00	654.0
421.00	1164.0
422.00	1643.0
423.10	11385.0
424.10	2515.0
425.10	342.0
441.10	30800.0
442.10	204544.0
443.10	38456.0
444.10	3331.0
445.00	197.0

Instrument :
BNA_M
ClientSampleId :
DFTPP001