
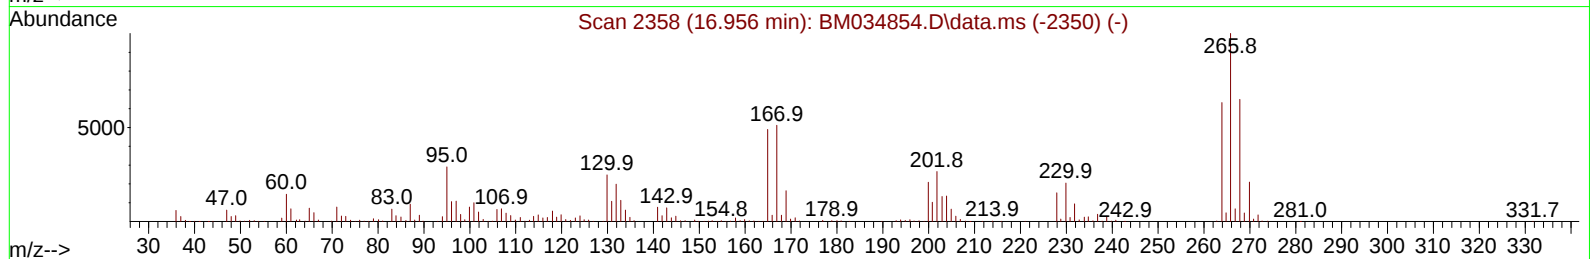
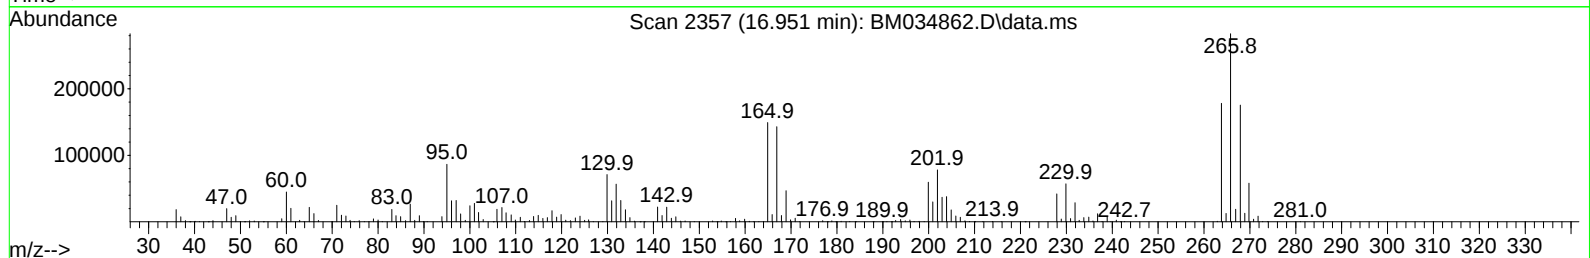


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034862.D
Acq On : 28 Apr 2022 12:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:04:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration

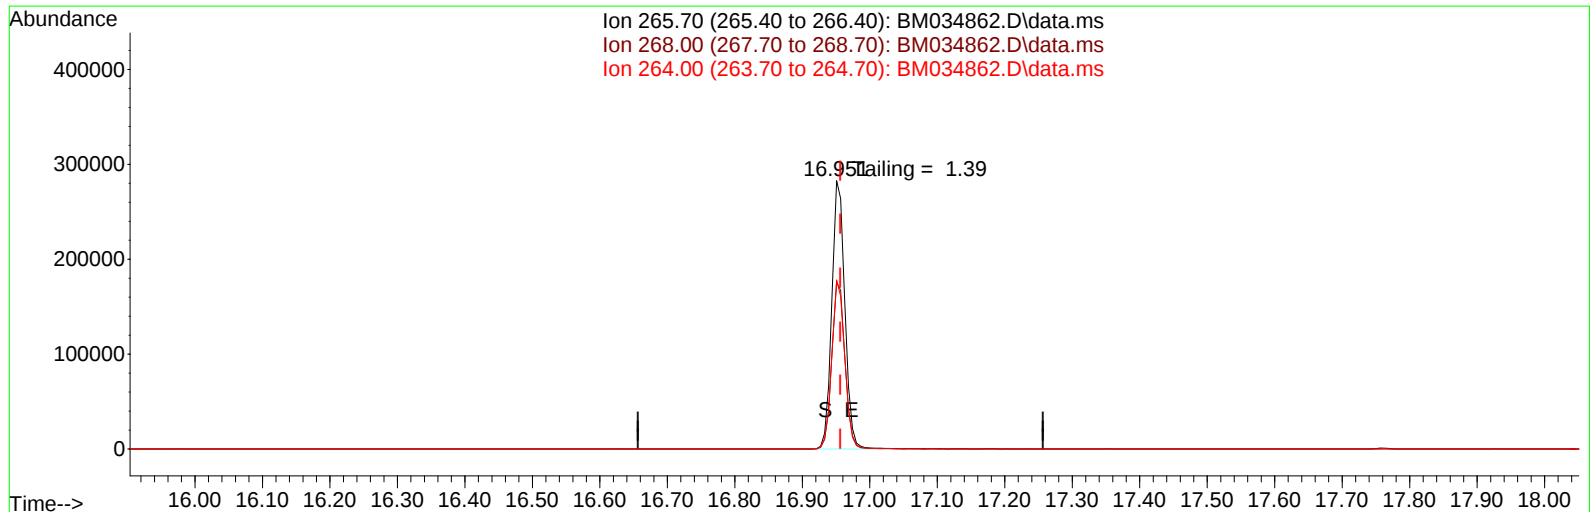

TIC: BM034862.D\data.ms

(70) Pentachlorophenol (C)




16.951min (-0.006) 980155.90 ng

response 380586

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.10
264.00	63.30	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034862.D
Acq On : 28 Apr 2022 12:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 29 06:04:44 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 28 01:51:59 2022
Response via : Initial Calibration

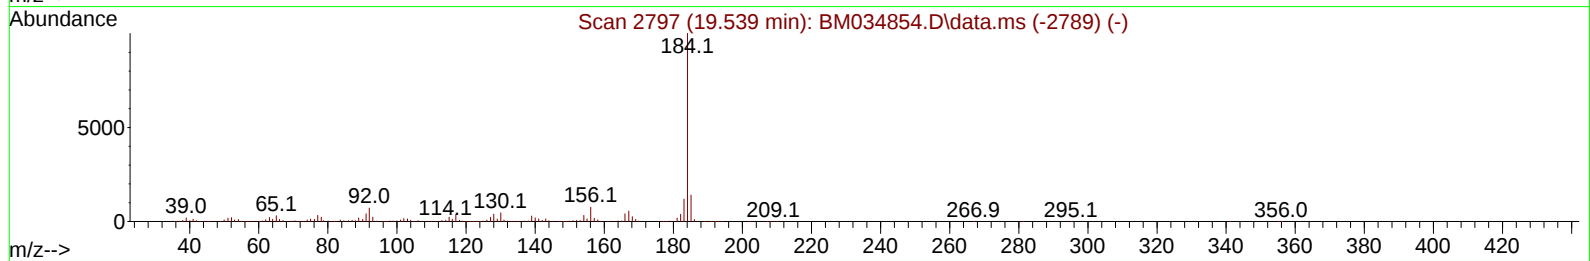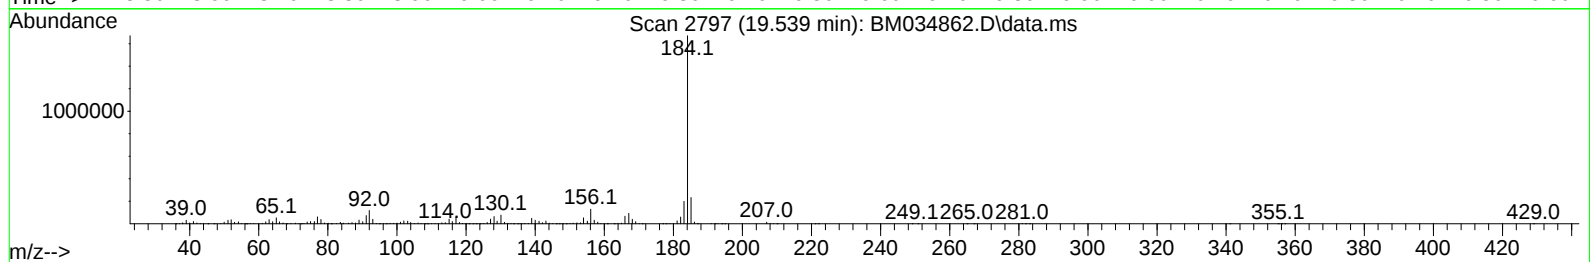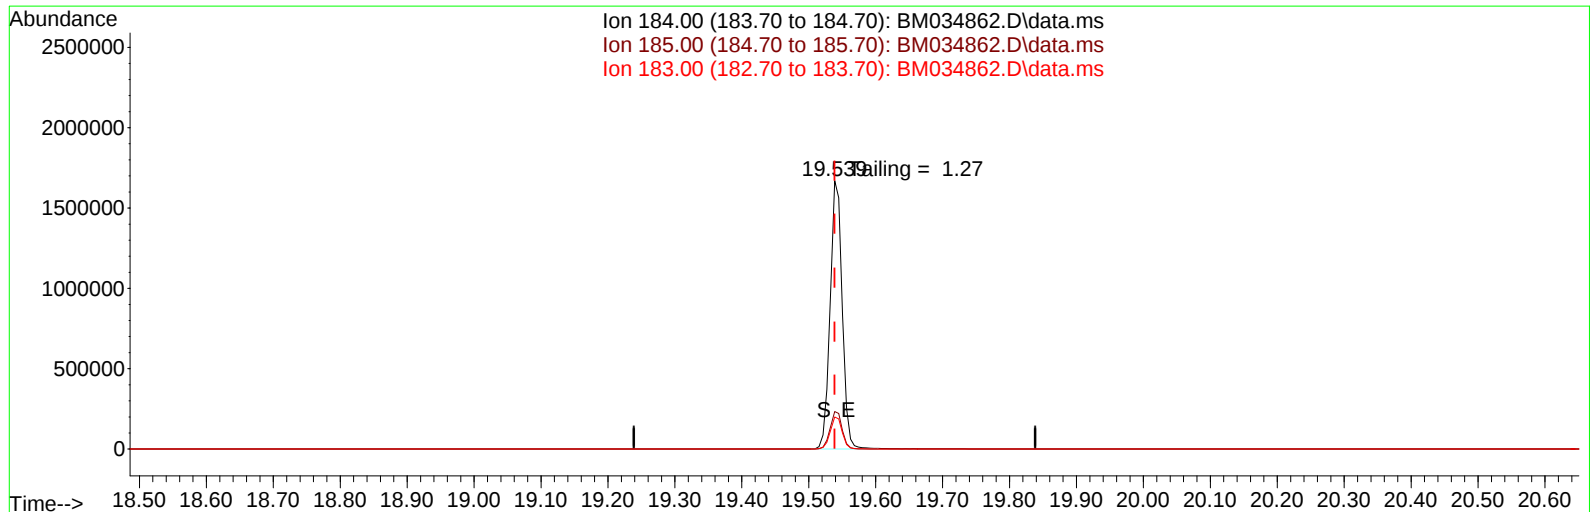

TIC: BM034862.D\data.ms

(77) Benzidine**19.539min (+ 0.000) 20256.51 ng****response 2102761**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.99
183.00	11.90	11.92
0.00	0.00	0.00