

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
 Data File : BM034864.D
 Acq On : 28 Apr 2022 13:22
 Operator : CG/JU
 Sample : PB144297BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB144297BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.505	404	411	422	rBV	5475440	7688557	63.03%	12.123%
2	7.099	673	682	699	rBV	4921413	7850082	64.36%	12.378%
3	7.928	817	823	833	rBV	948135	1515542	12.42%	2.390%
4	9.087	1012	1020	1032	rBV	3029383	5039501	41.31%	7.946%
5	10.734	1292	1300	1309	rBV	1224370	2019211	16.55%	3.184%
6	13.192	1711	1718	1725	rBV	7612202	10934017	89.64%	17.240%
7	14.563	1944	1951	1958	rBV	1689194	2460156	20.17%	3.879%
8	16.045	2196	2203	2216	rBV	5074487	6966072	57.11%	10.984%
9	17.304	2410	2417	2424	rBV	1844192	2603064	21.34%	4.104%
10	19.927	2857	2863	2868	rBV	10006345	12198078	100.00%	19.234%
11	21.480	3121	3127	3132	rBV	1683717	2207501	18.10%	3.481%
12	23.868	3527	3533	3543	rVB2	989218	1938847	15.89%	3.057%


Sum of corrected areas: 63420628

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034864.D
Acq On : 28 Apr 2022 13:22
Operator : CG/JU
Sample : PB144297BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144297BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

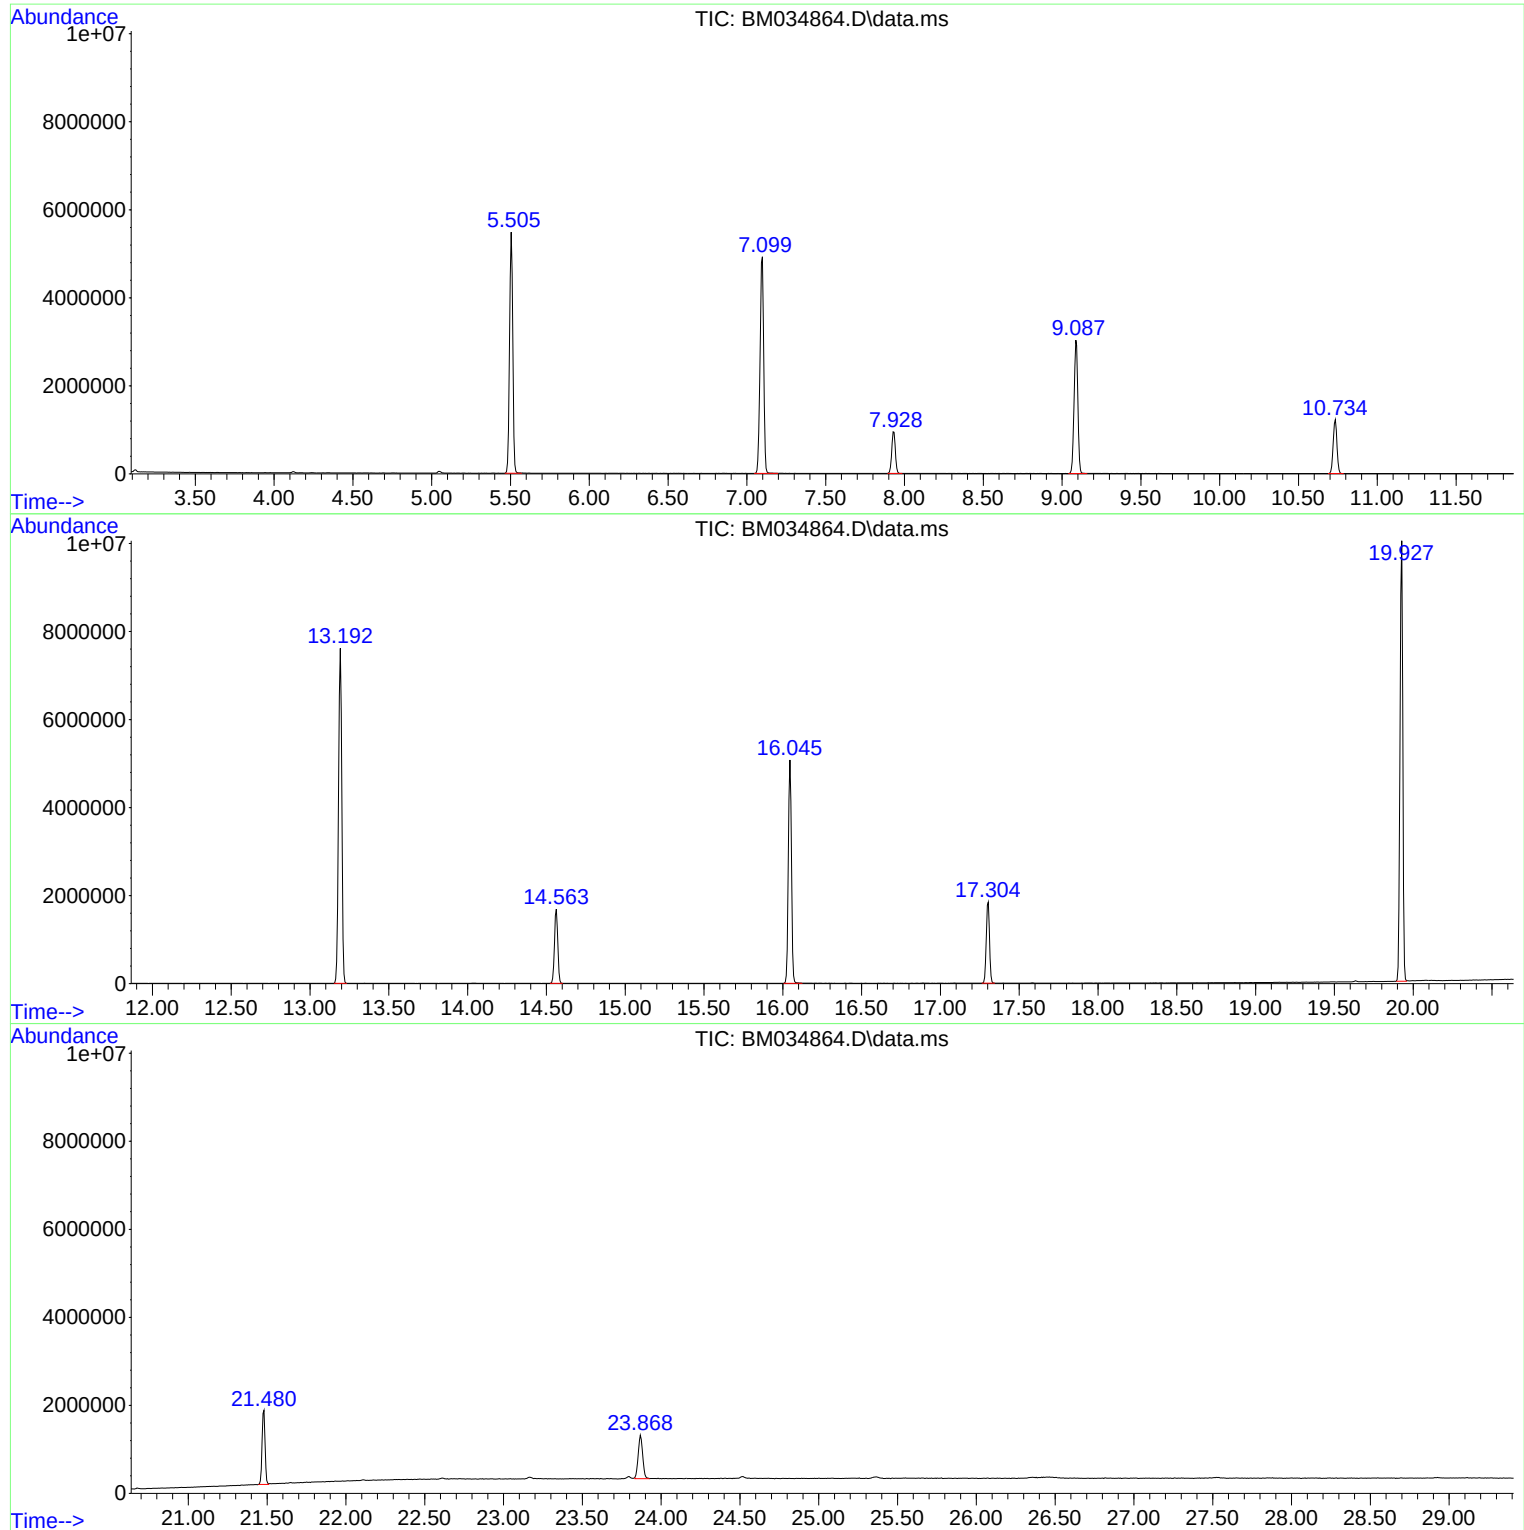

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034864.D
Acq On : 28 Apr 2022 13:22
Operator : CG/JU
Sample : PB144297BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144297BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042822\
Data File : BM034864.D
Acq On : 28 Apr 2022 13:22
Operator : CG/JU
Sample : PB144297BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB144297BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------